

A female scientist with blonde hair, wearing a white lab coat and safety glasses, is holding a round-bottom flask filled with a red liquid. She is looking directly at the camera. The background is a laboratory setting with shelves and windows.

# Competence in Labware

---

Labware range

# Welcome!

---

VITLAB has over 100 years of tradition. The company VITRI GmbH & Co. KG was established in 1908 in Mühlthal, and the laboratory division was spun off in 1989 as VITLAB. Today, VITLAB is one of the leading manufacturers of liquid handling instruments and performance plastic laboratory products for industrial and scientific applications. We develop and manufacture these laboratory products at our own production facility.

Our extensive range of products provides optimal support in your laboratory work in a wide variety of application ranges. Regardless of whether your work involves volume measurement, sampling or storage: VITLAB products will facilitate it while continuing to ensure that you achieve perfect results.

We hope that this new catalogue will serve as a valuable resource to aid in your lab work. We would be glad to respond to your enquiries, and look forward to receiving suggestions and ideas from our users.





This catalogue describes our products and provides all essential information. You will find detailed data regarding the various plastics clearly presented in the chapter entitled “General and Technical Information”. To simplify your search, our product range has been categorised into the following areas of application: dispensing, pipetting, titration, volume measurement, measuring and transferring, sample preparation, saving and storing, lab assistants.

Under “Volume Measurement”, for example, you will find a wide variety of classical volumetric instruments such as volumetric flasks, measuring cylinders, and associated accessories.

In addition to the range of products that appears in our catalogue, we also produce plastic products according to customer specification. For example, bottles and beakers required for special tasks can be commissioned with a specified geometry and thickness. Optionally, the products can be printed with an individualised scale or with customised labelling. Labware for promotional use can be designed and printed with a company name and logo. We can even accommodate requests for individualised packaging formats, materials, and designs. Further information is available in the VITLAB® Promotional chapter.

Many possibilities can be realised – don’t hesitate to ask what we can do for you!





# VITLAB

## Your reliable partner

---

### Certified quality

Independent inspections and routine internal audits guarantee the effectiveness of VITLAB's quality management system throughout the entire company, from development to shipment. As a result, the phrase 'Made by VITLAB' has become synonymous with quality.

Over 98% of our product line is made in Germany. Supplemental procedures such as tempering and volume testing are conducted in our own facilities, which guarantees the highest possible product quality

and measurement accuracy. Our continuous improvement paradigm supports our goal of 0% failure.

The VITLAB Quality Management System has been continuously certified since January 1994, according to DIN EN ISO 9001. Active stewardship of the environment is an equally strong pillar of our business philosophy. VITLAB has been certified according to DIN EN ISO 14001 since May, 1999.



## Prompt deliveries Competent customer service

The highly efficient logistics in the Großostheim production facility facilitate the shortest possible delivery times for all products listed in the catalogue. For the standard articles, we strive for an availability of over 94%.

Due to its intensive partnerships with distributors in over 70 countries, VITLAB can offer sound on-site advice, individual support, and quick answers to your questions. Our qualified product training sessions

provide comprehensive technical and application-oriented information on using our products. Should problems arise, our expert repair service keeps downtime as short as possible.

VITLAB products can be ordered from specialist dealers worldwide. Our authorised sales partners can be found on the internet at:

**[www.vitlab.com](http://www.vitlab.com)**

Or contact us directly.



# For your information

---



## Your contact Customer Service

Our Customer Service staff is at your service to provide you with competent advice and answers to all your queries and questions concerning offers, orders and deliveries. Our Product Management and Sales Team are at your disposal – also “on site” – with any technical information or assistance that you might require for your application.

### VITLAB GmbH, Customer Service

tel: +49 6026 9 77 99-0

fax: +49 6026 9 77 99-30


e-mail: [info@vitlab.com](mailto:info@vitlab.com)

web: [www.vitlab.com](http://www.vitlab.com)

Please understand that technical specifications, catalogue numbers and designs may change after this catalogue is published. The illustrations used are for representation only, and the details may vary from the description. All measurements, with the exception of exact tolerances, should be understood as approximate values. Please keep in mind that the actual testing and measuring results can be influenced by a variety of factors that are beyond our control. Therefore, you should carefully check the transferability of the data applying it to a particular application.

The packaging units (PU) correspond to the minimum order quantities. All up-to-date information is also available on the internet at [www.vitlab.com](http://www.vitlab.com).

If you need additional information, please call us.

**VITLAB**  , VITLAB<sup>®</sup>, maneus<sup>®</sup>,  
pipeo<sup>®</sup>, VITsafe<sup>™</sup>, VITgrip<sup>™</sup>  
are brands of VITLAB GmbH.

# Table of contents

---

## Dosing

Bottle-top dispensers and accessories

Starting on page 9

## Pipetting

Micropipettes, tips and accessories

Starting on page 21

## Titration

Bottle-top burettes, burettes and accessories

Starting on page 29

## Volume measurement

Volumetric flasks, graduated cylinders, pipettes, pipette helpers and accessories

Starting on page 35

## Measuring and transferring

Graduated beakers, scoops, spatula, forceps, funnels and accessories

Starting on page 55

## Sample preparation

Wash bottles, dropping bottles, dropping pipettes, spray bottles, Griffin beakers, watch glasses, Erlenmeyer flasks, magnetic stirring bars, mortars, pestles, equipment for material separation, desiccators, sample vials, staining cuvettes and accessories

Starting on page 65

## Saving and storing

Lab bottles, reagent bottles, storing bottles and transport containers

Starting on page 101

## Lab assistants

Connectors, valves, trays, drawer organisers and drying racks

Starting on page 117

## VITLAB<sup>®</sup> Promotional

Starting on page 125

## General and technical information

Starting on page 129



# Clear product statements

---

Our aim is to provide you with a clear and comprehensive presentation of all relevant product information. For quick reference, we use the following symbols:



DIN ISO-compliant Class A volumetric instruments



DE-M marking for conformity certified products according to the German Measurement and Calibration Regulation



Food-safe products according to EU Directive No. 10/2011



Products with high protection for light-sensitive substances



Products individually packaged in PE bags, labelled with the article number, description and EAN code



Products that can be autoclaved at 121 °C (2 bar) according to DIN EN 285. Note restrictions!



CE mark according to EU Guideline 2004/108/EC, 93/68/EEC; 73/23/EEC, and 93/68/EEC



CE-IVD mark according to EU Guideline 98/79/EC



# Perfection in Liquid Handling

HIGHEST RELIABILITY IN DISPENSING



## VITLAB® Dispenser line: genius<sup>2</sup>, simplex<sup>2</sup>, and TA<sup>2</sup>

VITLAB® genius<sup>2</sup> and simplex<sup>2</sup> bottle-top dispensers are a family of instruments with proven precision that offer many advantages in routine liquid-handling operations. VITLAB® genius<sup>2</sup> and simplex<sup>2</sup> instruments can be used for practically any task and are suitable for organic and inorganic solutions, while VITLAB® TA<sup>2</sup> dispensers have been specially developed for use in trace analysis and with highly concentrated media. As they are produced from materials with extremely high chemical resistance (e.g. PTFE, PFA, FEP, borosilicate glass and platinum-iridium), VITLAB® bottle-top dispensers are very robust and reliable and resistant against most acids, bases and organic solvents.



	VITLAB® genius <sup>2</sup> /simplex <sup>2</sup> /simplex <sup>2</sup> <sub>fix</sub>	VITLAB® TA <sup>2</sup>
Applications	Salt solutions, acids, bases, and many organic solvents	Specially for use in trace analysis for dispensing high-purity and highly concentrated acids and alkalis, as well as hydrogen peroxide, bromine and HF
Components in contact with media	Borosilicate glass, Al <sub>2</sub> O <sub>3</sub> -ceramic, FEP, ETFE, PFA, PTFE, platinum-iridium, PP (screw cap)	Various fluoroplastics (e.g., ETFE, FEP, PFA, PCTFE, PTFE), Al <sub>2</sub> O <sub>3</sub> -sapphire, platinum-iridium or tantalum (depending on the model)
Operating limits	Temperature: +15 °C to +40 °C Steam pressure: max. 600 mbar Viscosity: max. 500 mm <sup>2</sup> /s Density: max. 2.2 g/cm <sup>3</sup>	Temperature: +15 °C to +40 °C Steam pressure: max. 600 mbar Viscosity: max. 500 mm <sup>2</sup> /s Density: max. 3.8 g/cm <sup>3</sup>

\* Dynamic viscosity [mPas] = kinematic viscosity [mm<sup>2</sup>/s] x density [g/cm<sup>3</sup>]

General guide for dispenser selection (for the classification of dispenser media, see page 11).

Salt solutions	Acids and bases	Solvents	High-purity and highly concentrated acids and bases	Hydrofluoric acid (HF), bromine, hydrogen peroxide
VITLAB® genius <sup>2</sup> /simplex <sup>2</sup>		VITLAB® genius <sup>2</sup> /simplex <sup>2</sup>		
			VITLAB® TA <sup>2</sup>	

# Dosing

## Recommended usage ranges for VITLAB® genius<sup>2</sup> / simplex<sup>2</sup> / simplex<sup>2</sup><sub>fix</sub>:

Medium	Medium	Medium
<input type="radio"/> Acetaldehyde	<input type="checkbox"/> Copper sulphate	<input type="radio"/> Methyl butyl ether
<input type="radio"/> Acetic acid, ≤ 96%	<input type="radio"/> Cresol	<input type="radio"/> Methyl ethyl ketone
<input type="radio"/> Acetone	<input type="radio"/> Cumene (Isopropylbenzene)	<input type="radio"/> Methyl formate
<input type="radio"/> Acetonitrile	<input type="radio"/> Cyclohexanone	<input type="radio"/> Methyl propyl ketone
<input type="radio"/> Acetylacetone	<input type="radio"/> Decane	<input type="radio"/> Mineral oil (Motor oil)
<input type="radio"/> Acrylic acid	<input type="radio"/> 1-Decanol	<input type="radio"/> Monochloroacetic acid, ≤ 50%
<input type="radio"/> Acrylonitrile	<input type="radio"/> Diethylene glycol	<input type="checkbox"/> Nitric acid, ≤ 60% */**
<input type="radio"/> Adipic acid	<input type="radio"/> Dibenzyl ether	<input type="radio"/> Nitrobenzene
<input type="radio"/> Allyl alcohol	<input type="radio"/> Dichlorobenzene	<input type="radio"/> Octane
<input type="checkbox"/> Aluminium chloride	<input type="radio"/> Dichloroethane	<input type="radio"/> Oleic acid
<input type="radio"/> Amino acid	<input type="radio"/> Dichloromethane	<input type="radio"/> Oxalic acid
<input type="checkbox"/> Ammonia solution, ≤ 20%	<input type="radio"/> Diethanolamine	<input type="checkbox"/> Perchloric acid
<input type="checkbox"/> Ammonium chloride	<input type="radio"/> Diethyl ether	<input type="radio"/> Petroleum
<input type="checkbox"/> Ammonium fluoride	<input type="radio"/> Diethylamine	<input type="radio"/> Phenol
<input type="checkbox"/> Ammonium hydroxide, ≤ 20%	<input type="radio"/> 1,2 Diethylbenzene	<input type="radio"/> Phenylethanol
<input type="checkbox"/> Ammonium sulphate	<input type="radio"/> Dimethyl sulphoxide (DMSO)	<input type="radio"/> Phenylhydrazine
<input type="radio"/> Amyl acetate	<input type="radio"/> Dimethylaniline	<input type="checkbox"/> Phosphoric acid, ≤ 85%
<input type="radio"/> Amyl alcohol (Pentanol)	<input type="radio"/> Dimethylformamide (DMF)	<input type="checkbox"/> Phosphoric acid, 85% + sulphuric acid, 98%, 1:1
<input type="radio"/> Amyl chloride (Chloropentane)	<input type="radio"/> 1,4 Dioxane	<input type="radio"/> Piperidine
<input type="radio"/> Aniline	<input type="radio"/> Diphenyl ether	<input type="checkbox"/> Potassium chloride
<input type="checkbox"/> Barium chloride	<input type="radio"/> Ethanol	<input type="checkbox"/> Potassium dichromate
<input type="radio"/> Benzaldehyde	<input type="radio"/> Ethanolamine	<input type="checkbox"/> Potassium hydroxide
<input type="radio"/> Benzene	<input type="radio"/> Ethyl acetate	<input type="checkbox"/> Potassium permanganate
<input type="radio"/> Benzoyl chloride	<input type="radio"/> Formaldehyde, ≤ 40%	<input type="radio"/> Propanol
<input type="radio"/> Benzyl alcohol	<input type="radio"/> Formamide	<input type="radio"/> Propionic acid
<input type="radio"/> Benzyl chloride	<input type="radio"/> Formic acid, ≤ 100%	<input type="radio"/> Propylene glycol (Propanediol)
<input type="radio"/> Benzylamine	<input type="radio"/> Gasoline	<input type="radio"/> Propylene oxide
<input type="checkbox"/> Boric acid, ≤ 10%	<input type="radio"/> Glacial acetic acid	<input type="radio"/> Pyridine
<input type="radio"/> Bromobenzene	<input type="radio"/> Glycerine	<input type="radio"/> Pyruvic acid
<input type="radio"/> Bromonaphthalene	<input type="radio"/> Glycol (Ethylene glycol)	<input type="radio"/> Salicylaldehyde
<input type="radio"/> Butanediol	<input type="radio"/> Glycolic acid, ≤ 50%	<input type="radio"/> Salicylic acid
<input type="radio"/> 1-Butanol	<input type="radio"/> Heating oil (Diesel oil)	<input type="radio"/> Silver acetate
<input type="radio"/> n-Butyl acetate	<input type="radio"/> Hexane	<input type="checkbox"/> Silver nitrate
<input type="radio"/> Butyl methyl ether	<input type="radio"/> Hexanoic acid	<input type="radio"/> Sodium acetate
<input type="radio"/> Butylamine	<input type="radio"/> Hexanol	<input type="checkbox"/> Sodium chloride
<input type="radio"/> Butyric acid	<input type="checkbox"/> Hydrochloric acid, ≤ 37% **	<input type="checkbox"/> Sodium dichromate
<input type="checkbox"/> Calcium carbonate	<input type="checkbox"/> Hydroiodic acid, ≤ 57% **	<input type="checkbox"/> Sodium fluoride
<input type="checkbox"/> Calcium chloride	<input type="checkbox"/> Iodine / potassium iodide solution	<input type="checkbox"/> Sodium hydroxide, ≤ 30%
<input type="checkbox"/> Calcium hydroxide	<input type="radio"/> Isoamyl alcohol	<input type="checkbox"/> Sodium hypochlorite
<input type="checkbox"/> Calcium hypochlorite	<input type="radio"/> Isobutanol	<input type="checkbox"/> Sulphuric acid, ≤ 98%
<input type="radio"/> Chloroacetaldehyde, ≤ 45%	<input type="radio"/> Isopropanol (2-propanol)	<input type="radio"/> Tartaric acid
<input type="radio"/> Chloroacetic acid	<input type="radio"/> Isopropyl ether	<input type="radio"/> Tetramethylammonium hydroxide
<input type="radio"/> Chloroacetone	<input type="radio"/> Lactic acid	<input type="radio"/> Toluene
<input type="radio"/> Chlorobenzene	<input type="checkbox"/> Magnesium chloride	<input type="radio"/> Turpentine
<input type="radio"/> Chlorobutane	<input type="checkbox"/> Mercury chloride	<input type="radio"/> Urea
<input type="radio"/> Chloronaphthalene	<input type="radio"/> Methanol	<input type="radio"/> Xylene
<input type="checkbox"/> Chromic acid, ≤ 50%	<input type="radio"/> Methoxybenzene	<input type="checkbox"/> Zinc chloride, ≤ 10%
<input type="checkbox"/> Chromic-sulphuric acid	<input type="radio"/> Methyl benzoate	<input type="checkbox"/> Zinc sulphate, ≤ 10%

The above data have been carefully checked and reflect the current state of knowledge. Always follow the instructions for use that accompany the instrument as well as the reagent manufacturer's instruction manual. In addition to the chemicals listed above, solutions of a wide variety of organic or inorganic salts (e.g., biological buffers), biological detergents, and cell culture media can be dispensed. Should you require information on chemicals not listed, please do not hesitate to contact us. Last updated: 09/17.

\* Use ETFE/PTFE bottle adapter

\*\* Use drying tube

Inorganic media

Organic media

## VITLAB® genius<sup>2</sup> / simplex<sup>2</sup> / simplex<sub>fix</sub><sup>2</sup>

VITLAB® dispensers are practically universally applicable and can be used with many **organic and inorganic solutions**. The materials that come into contact with media (borosilicate glass, Al<sub>2</sub>O<sub>3</sub> ceramics, FEP, ETFE, PFA, PTFE, platinum iridium and PP) are resistant to most acids, solvents and bases.

The devices are equipped with a positive displacement piston and a fluoroplastic (PFA) sealing lip on the cylinder wall. This latter acts like a windscreen wiper to **prevent crystal build-up on the cylinder wall** from readily crystallisable media. The glass cylinder is also coated with a plastic material that reduces the risk of splashes should breakage occur. The telescopic filling tube can be adjusted smoothly to different bottle heights.

The practical screwing mechanism and inner toothed bar enable a fast and precise volume adjustment (simplex<sup>2</sup> and genius<sup>2</sup>). The simple-to-use calibration function helps meet all the requirements for test equipment monitoring with minimal downtime. Reagent loss while bleeding is avoided with the innovative recirculation valve (only genius<sup>2</sup>). The screwable discharge valve is equipped with an additional safety bulb and closes the dosing channel, if dispensing tube is not installed, so that no medium can escape.

VITLAB® genius<sup>2</sup>, simplex<sup>2</sup> and simplex<sub>fix</sub><sup>2</sup> are completely autoclavable at 121 °C (2 bar) according to DIN EN 285 and DE-M marked.

Also available with DAkkS calibration certificate or individual certificate (at additional cost).



## VITLAB® genius<sup>2</sup>



Bottle-top dispenser with variable volume and recirculation system. DE-M marked.

Included in delivery: VITLAB® genius<sup>2</sup> (GL 45 thread), 3 or 5 thread adapters\* made of PP, telescopic filling tube, recirculation tube, mounting tool, quality certificate and operating manual.

Volume ml	Graduation ml	A** ≤ ± %	A** ≤ ± µl	CV** ≤ %	CV** ≤ µl	PU	Cat. No.
0.2 - 2.0	0.05	0.5	10	0.1	2	1	1625503
0.5 - 5.0	0.10	0.5	25	0.1	5	1	1625504
1.0 - 10.0	0.20	0.5	50	0.1	10	1	1625505
2.5 - 25.0	0.50	0.5	125	0.1	25	1	1625506
5.0 - 50.0	1.00	0.5	250	0.1	50	1	1625507
10.0 - 100.0	1.00	0.5	500	0.1	100	1	1625508

\* Nominal volume 2 - 10 ml: with adapters GL 25, GL 28, GL 32, GL 38, S 40 and telescopic intake tube (length 125 - 240 mm).  
Nominal volume 25 - 100 ml: with adapters GL 32, GL 38, S 40 and telescopic intake tube (length 170 - 330 mm).

\*\* Error tolerance conforming to DIN EN ISO 8655-5, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing. DE-M marked.



# Dosing

## VITLAB® simplex<sup>2</sup>



Bottle-top dispenser with variable volume. DE-M marked.

Included in delivery: VITLAB® simplex<sup>2</sup>, 3 respectively 5 thread adapters\* made of PP, telescopic filling tube, mounting tool, quality certificate and operating manual.

Volume ml	Graduation ml	A** ≤ ± %	A** ≤ ± µl	CV** ≤ %	CV** ≤ µl	PU	Cat. No.
0.2 - 2.0	0.05	0.5	10	0.1	2	1	1621503
0.5 - 5.0	0.10	0.5	25	0.1	5	1	1621504
1.0 - 10.0	0.20	0.5	50	0.1	10	1	1621505
2.5 - 25.0	0.50	0.5	125	0.1	25	1	1621506
5.0 - 50.0	1.00	0.5	250	0.1	50	1	1621507
10.0 - 100.0	1.00	0.5	500	0.1	100	1	1621508

\* Nominal volume 2 - 10 ml: with adapters GL 25, GL 28, GL 32, GL 38, S 40 and telescopic intake tube (length 125 - 240 mm).

Nominal volume 25 - 100 ml: with adapters GL 32, GL 38, S 40 and telescopic intake tube (length 170 - 330 mm).

\*\* Error tolerance conforming to DIN EN ISO 8655-5, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing. DE-M marked.



## VITLAB® simplex<sup>2</sup><sub>fix</sub>



Bottle-top dispenser with fixed volume. DE-M marked.

Included in delivery: VITLAB® simplex<sup>2</sup>, 3 or 5 thread adapters\* made of PP, telescopic filling tube, mounting tool, quality certificate and operating manual.

Volume ml	Graduation ml	A** ≤ ± %	A** ≤ ± µl	CV** ≤ %	CV** ≤ µl	PU	Cat. No.
1.0	-	1.0	10	0.2	2	1	1622502
5.0	-	0.5	25	0.1	5	1	1622504
10.0	-	0.5	50	0.1	10	1	1622505

\* Nominal volume 1 - 10 ml: with adapters GL 25, GL 28, GL 32, GL 38, S 40 and telescopic intake tube (length 125 - 240 mm).

\*\* Error tolerance conforming to DIN EN ISO 8655-5, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing. DE-M marked.





## VITLAB® TA<sup>2</sup>



The VITLAB® TA<sup>2</sup> dispenser is the dosing device of choice to meet the demanding purity standards required in trace analysis. The high quality parts that come exclusively in contact with the medium and the specially developed and proven cleaning process to be done before use results in **a reduced release of trace metal ions to the low ppb range, or, depending on the application, even the ppt range**. The parts that are in contact with media are made of various fluoroplastics (e.g. ETFE, FEP, PFA, PTFE, PCTFE), Al<sub>2</sub>O<sub>3</sub>-sapphire, platinum-iridium or tantalum (depending on model).

Thanks to the excellent chemical resistance of the materials used, the new dispenser can also be deployed with **highly concentrated acids and bases**, such as perchloric, sulphuric and nitric acid. Depending on the application, there is a choice of two different valve spring systems: the VITLAB® TA<sup>2</sup> with tantalum spring is recommended for dosing of hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>). For applications using sodium hydroxide (up to a max. concentration of 30%) or hydrogen fluoride (HF) the platinum-iridium spring is recommended. In order to minimize the loss of valuable reagents or sample solutions, VITLAB offers the dispenser with the optional recirculation valve. The practical screwing mechanism and inner toothed bar enable a fast, easy and precise volume adjustment. Also available with DAKKS calibration certificate (at additional cost).

Included in delivery:

VITLAB® TA<sup>2</sup> dispenser (thread GL 45), 3 bottle adapters (GL 28/S 28 (ETFE), GL 32 (ETFE) and S 40 (PTFE), telescopic filling tube, recirculation valve (optionally), mounting tool, quality certificate and operating manual.

Volume ml	Valve spring	Recircu- lation	Graduation ml	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
1.0 - 10.0	Pt-Ir	no	0.2	0.5	0.1	1	1627515
1.0 - 10.0	Pt-Ir	yes	0.2	0.5	0.1	1	1627525
1.0 - 10.0	Ta	no	0.2	0.5	0.1	1	1627535
1.0 - 10.0	Ta	yes	0.2	0.5	0.1	1	1627545

\* Error tolerance conforming to DIN EN ISO 8655-5, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing. DE-M marked.

## Recommended dispensing media for VITLAB® TA<sup>2</sup>

Dispensing medium	Valve spring: Pt-Ir	Valve spring: Ta
Acetic acid	+	+
Ammonia solution	+	+
Bromine	+	+
Hydrochloric acid	+	+
Hydrofluoric acid*	+	-
Hydrogen peroxide	-	+
Nitric acid	+	+
Perchloric acid	+	+
Phosphoric acid	+	+
Sodium hydroxide, 30%	+	-
Sulphuric acid	+	+
Water	+	+

+ suitable / - unsuitable

\* Note: Hydrofluoric acid reacts slightly with sapphire resulting in slightly increased aluminium levels. To reduce these values we recommend discarding 3-5 dosings of 2 ml each before performing analysis.

# Dosing

## Brown glass bottles for VITLAB® genius<sup>2</sup> and simplex<sup>2</sup>

Threaded brown glass (soda lime glass) bottles with an ethylene acrylate coating for increased safety, and a screw cap. The plastic coating significantly reduces hazardous glass splintering during breakage. The maximum working temperature for coated bottles is 80 °C. To preserve the coating, do not clean at temperatures exceeding 60 °C.

Volume ml	Form	Thread GL	PU	Cat. No.
250	square	32	1	1671515
500	square	32	1	1671520
1000	square	45	1	1671500
2500	round	45	1	1671510



Suitable plastic bottles can be found starting on page 103.

## Plastic stand for VITLAB® dispensers

For secure anchoring, made entirely of polypropylene for contamination-free operation (no metal). Suitable for VITLAB® dispensers with screw coupling GL 45.

Stand rod: 300 mm; base: 220 x 160 mm; weight: 1,130 g.

Description	PU	Cat. No.
Plastic stand	1	1671116




## Drying tube for VITLAB® dispensers

PP, transparent, unfilled, with sealing ring (PTFE).

Can directly be connected to every dispenser.

Description	PU	Cat. No.
Drying tube, PP, unfilled	1	1671090

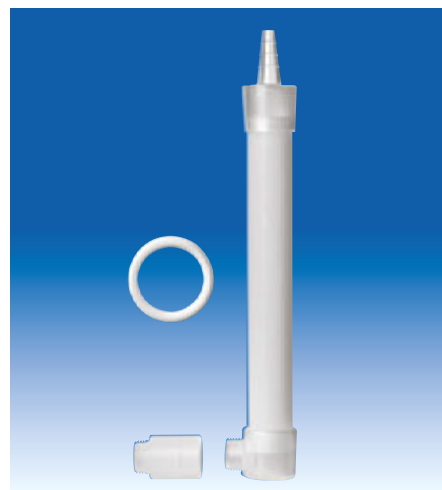



## Flexible discharge tubes for VITLAB® dispensers

Coiled, made of FEP, approx. 80 cm length, with handle and recirculation valve made of PTFE. Includes handle and assembly instructions. Not suitable for hydrofluoric acid (HF)!

Description	PU	Cat. No.
Flexible discharge tube for genius <sup>2</sup> / simplex <sup>2</sup> 2, 5 and 10 ml	1	1678132
Flexible discharge tube for genius <sup>2</sup> / simplex <sup>2</sup> 25, 50 and 100 ml	1	1678134
Flexible discharge tube for VITLAB® TA <sup>2</sup> (with grey lever)	1	1678136



PP adapter

## Adapter for VITLAB® dispensers

For securely screwing the dispenser onto the reagent bottles with an NS neck, GL screw threading or an S buttress thread. For VITLAB® TA<sup>2</sup> please use adapter ETFE/PTFE. These are recommended for VITLAB® genius<sup>2</sup> and simplex<sup>2</sup> when an increased resistance to chemicals is required (see media table pg. 11).

Description	External thread	Bottle neck threads	PU	Cat. No.
NS-adapter, PP	GL 32	NS 19/26	1	1670066
NS-adapter, PP	GL 32	NS 24/29	1	1670067
NS-adapter, PP	GL 32	NS 29/32	1	1670068
Thread adapter, PP	GL 32	GL 25	1	1670150
Thread adapter, PP	GL 32	GL 28	1	1670155
Thread adapter, PP	GL 32	GL 38	1	1670165
Thread adapter, PP	GL 32	GL 45	1	1670175
Thread adapter, PP	GL 32	S 40	1	1670170
Thread adapter, PP	GL 45	GL 32	1	1670180
Thread adapter, PP	GL 45	GL 38	1	1670110
Thread adapter, PP	GL 45	S 40	1	1670120
Thread adapter, ETFE	GL 32	GL 25	1	1670072
Thread adapter, ETFE	GL 32	GL 28	1	1670080
Thread adapter, ETFE	GL 32	GL 45	1	1670105
Thread adapter, ETFE	GL 45	GL 32	1	1670100
Thread adapter, ETFE	GL 45	GL 38	1	1670115
Thread adapter, PTFE	GL 45	S 40	1	1670125



ETFE adapter



# Dosing

## Telescopic filling tubes for VITLAB® dispensers

Telescopic filling tube made of FEP, ETFE and PTFE.

Suitable for dispenser with nominal volume	Outer-Ø mm	Length mm	PU	Cat. No.
2/5/10 ml	6.0	70-140	1	1678210
2/5/10 ml	6.0	125-240	1	1678212
2/5/10 ml	6.0	195-350	1	1678214
2/5/10 ml	6.0	250-480	1	1678216
25/50/100 ml	7.6	170-330	1	1678218
25/50/100 ml	7.6	250-480	1	1678220



## Sealing ring for the valve block for VITLAB® dispensers

Sealing ring for valve block made of PTFE for dosing highly volatile media.

Description	PU	Cat. No.
Sealing ring for valve block	1	1671683



## Ventilation plug for micro filter for VITLAB® genius<sup>2</sup> and simplex<sup>2</sup>

PP, with Luer-cone and sealing ring (PTFE).

Description	PU	Cat. No.
Ventilation plug for micro filter	1	1671682



## Dispensing cartridge for VITLAB® TA<sup>2</sup>

Calibrated, including safety ring, with quality certificate. Nominal volume 10 ml.

Description	PU	Cat. No.
Dispensing cartridge	1	1670702





## VITLAB® piccolo

For dispensing tiny quantities of liquids in all areas of biochemical and medical research.

Even the **smallest quantities can be dispensed directly from the bottle** with the VITLAB® piccolo - a big help, particularly for serial dispensing operations. Special advantage: Pipette tips are unnecessary. This reduces costs.

The ergonomic design makes dispensing effortless and stress-free. The VITLAB® piccolo **can be operated with only one hand**. Use the thumb to depress the volume dispensing button, just as with a pipette, and a reset mechanism refills the volume automatically.

The discharge tube can be rotated over 360° so that it is always optimally situated with respect to the bottle label.

The VITLAB® bottle-top dispensers piccolo 1 and piccolo 2 are used mainly in connection with aqueous and highly diluted agents.

VITLAB® piccolo 1 with a fixed volume

VITLAB® piccolo 2 with two fixed volumes

Included in delivery:

VITLAB® piccolo 1 or 2 (GL 28 threads), mounting tool and operating manual.

Type	Volume µl	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
piccolo 1	100	3.0	0.4	1	1610501
piccolo 1	200	2.5	0.4	1	1610502
piccolo 1	250	2.0	0.4	1	1610503
piccolo 1	500	1.5	0.3	1	1610504
piccolo 1	1000	1.0	0.2	1	1610506
piccolo 2	100 / 250	2.0	0.4	1	1611503
piccolo 2	500 / 1000	1.0	0.2	1	1611506
piccolo 2	1000 / 2000	1.0	0.2	1	1611508

\* Error tolerance conforming to DIN EN ISO 8655-5, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing.

# Dosing

## Adapter for VITLAB® piccolo

For securely screwing the dispenser onto reagent bottles with GL screw threading.

Description	External thread	Bottle neck threads	PU	Cat. No.
Thread adapter, PP	GL 28	GL 32	1	1670145



## Bottles for VITLAB® piccolo, PE-HD

Transparent. With screw cap made of PP. Space-saving due to the square cross-section and the high shoulders.

Volume ml	Thread	Height mm	Dimension mm	PU	Cat. No.
100	GL 32	78	46 x 46	24	92489
250	GL 28	80	80 x 80	24	91989
500	GL 32	106	90 x 90	12	92089
1000	GL 32	187	80 x 80	12	92189



## Brown glass bottles for VITLAB® piccolo

Threaded brown glass (soda lime glass) bottles with an ethylene acrylate coating for increased safety, and a screw cap. The plastic coating significantly reduces hazardous glass splintering during breakage. The maximum working temperature for coated bottles is 80 °C. To preserve the coating, do not clean at temperatures exceeding 60 °C.

Volume ml	Form	Thread GL	PU	Cat. No.
100	round	28	1	1671505
100	square	32	1	1671506







# Perfection in Liquid Handling

PRECISE AND CONVENIENT PIPETTING





## VITLAB® micropipette



The VITLAB® piston-operated pipettes are the ideal manual pipettes for demanding laboratory applications, and have all the features required by users: robust, with ergonomic shape and simple operation, completely autoclavable, highly accurate with simple calibration for long-lasting reliability.

The large, central pipetting button provides a uniform and smooth movement of the piston. For rapid replacement of the tips, the ergonomic eject button is placed easily accessible to the thumb on the front side. The VITLAB® micropipette is easy to use for both right- and left-handers. The 4-digit volume display with integrated zoom function and vertical arrangement of the numbers (top to bottom reading direction) ensures an **optimal readability of the volume** at all times. The desired volume can be set by rotating the volume-setting wheel with ease and precision. The clearly visible colour-coded frame of the volume display allows easy selection of the right pipette tip.

If necessary, e.g. for applications with non-aqueous solutions, the **integrated calibration function allows an adjustment without tools directly in the laboratory**. The corrosion-resistant piston and ejector ensure a long product life.

The micropipette is DE-M marked, CE-IVD compliant and is completely autoclavable at 121 °C (2 bar) according to DIN EN 285. Also available with DAkKS calibration certificate (at additional cost).

Included in delivery: VITLAB® micropipette, silicone grease, sample bag with pipette tips, quality certificate, and operating manual.

Volume µl	A* ≤ ± %	A* ≤ ± µl	CV* ≤ %	CV* ≤ µl	Tip µl	PU	Cat. No.
0.5 - 10	1.0	0.1	0.5	0.05	20	1	1641000
2 - 20	0.8	0.16	0.4	0.08	200	1	1641002
10 - 100	0.6	0.6	0.2	0.2	200/300	1	1641004
20 - 200	0.6	1.2	0.2	0.4	200/300	1	1641006
100 - 1000	0.6	6	0.2	2	1000	1	1641008
500 - 5000	0.6	30	0.2	10	5000	1	1641010
1000 - 10000	0.6	60	0.2	20	10000	1	1641012

\* Calibrated to deliver ,Ex'. \* Accuracy and coefficient of variation based on the nominal volume (= maximum volume) printed on the instrument, if instrument, environment and distilled water are at the same temperature (20 °C), as well as uniform, jerk-free handling. The margins of error are under those specified in DIN EN ISO 8655-2. DE-M marked.

# Pipetting

## VITLAB® micropipette -8 / -12



The VITLAB® micropipettes -8 and -12 are characterized by their especially user-friendly operation while pipetting long series. They have all the features required by users: robust, completely autoclavable and highly accurate, with simple calibration for long lasting reliability, especially for established multichannel pipette applications, such as immunological assays, dilution series, or use with cell cultures in microtiter plates.

By using innovative plastic materials, the VITLAB® multichannel pipettes are **at the same time very robust and light-weight**. To ensure a long operating life, the plastic materials used are corrosion-resistant. The ergonomic finger rest coupled with the low weight contribute to comfortable handling of the pipettes. To provide an optimal and comfortable working position, the manifold can be rotated freely 360° in both directions.

The large, central pipetting button provides uniform and smooth movement of the piston. In addition, the short stroke of 12.5 mm reduces the risk of muscular disorders as a consequence of repeated stress, such as "Repetitive Strain Injury Syndrom" (RSI). The combination of the stepped design of the ejector and special rings made of FKM reduce the effort needed for ejecting the tips and thus provide comfortable operation of the pipette.

The multichannel pipettes are **especially service-friendly** for care and maintenance, as well as for calibration. If necessary, e.g. for applications with non-aqueous solutions, the integrated calibration function allows an adjustment without tools directly in the laboratory. Single shafts and seals can be easily removed, and thus can be directly cleaned or replaced.

The VITLAB® micropipette -8 and -12 are DE-M marked, CE-IVD compliant, and are completely autoclavable at 121 °C (2 bar) according to DIN EN 285. Also available with DAkKS calibration certificate or individual quality certificate (at additional cost).

Included in delivery: VITLAB® micropipette -8 or -12, mounting tool for nose cones, silicone grease, 8 or 12 V-rings including instructions and mounting plus demounting tool, quality certificate and operating manual.

Volume µl	A* ≤ ± %	A* ≤ ± µl	CV* ≤ %	CV* ≤ µl	Tip µl	PU	Cat. No.
micropipette -8							
0.5 - 10	1.6	0.16	1.0	0.1	20	1	1608000
5 - 50	0.8	0.4	0.4	0.2	200	1	1608002
10 - 100	0.8	0.8	0.3	0.3	200/300	1	1608004
20 - 200	0.8	1.6	0.3	0.6	200/300	1	1608006
30 - 300	0.6	1.8	0.3	0.9	300	1	1608008
micropipette -12							
0.5 - 10	1.6	0.16	1.0	0.1	20	1	1612000
5 - 50	0.8	0.4	0.4	0.2	200	1	1612002
10 - 100	0.8	0.8	0.3	0.3	200/300	1	1612004
20 - 200	0.8	1.6	0.3	0.6	200/300	1	1612006
30 - 300	0.6	1.8	0.3	0.9	300	1	1612008

\* Calibrated to deliver 'Ex'. Accuracy (A) and Coefficient of variation (CV) refer to the nominal capacity (= maximum volume) indicated on the instrument, obtained with instrument and distilled water at equilibrium with ambient temperature at 20 °C, and with smooth, steady operation. The error limits are under those specified in DIN EN ISO 8655-2. DE-M marked.



## VITLAB® micropipette Starter-Sets

Each VITLAB® Starter Set includes 3 variable VITLAB® micropipettes with different volumes and associated, color-coded tip boxes, as well as 3 rack mounts for appropriate storage of your new VITLAB® micropipettes.

Our micropipettes are DE-M marked, CE-IVD compliant and are completely autoclavable at 121 °C (2 bar) according to DIN EN 285.



### Starter Set "Mini"

Scope of delivery:

- VITLAB® micropipette 0.5 - 10 µl
- VITLAB® micropipette 10 - 100 µl
- VITLAB® micropipette 100 - 1000 µl
- Tip-Box 0.5 - 20 µl
- Tip-Box 2 - 200 µl
- Tip-Box 50 - 1000 µl
- Rack mount (3x)

Cat. No.: 33331

### Starter Set "Classic"

Scope of delivery:

- VITLAB® micropipette 2 - 20 µl
- VITLAB® micropipette 20 - 200 µl
- VITLAB® micropipette 100 - 1000 µl
- Tip-Box 2 - 200 µl (2x)
- Tip-Box 50 - 1000 µl
- Rack mount (3x)

Cat. No.: 33332

### Starter Set "Maxi"

Scope of delivery:

- VITLAB® micropipette 100 - 1000 µl
- VITLAB® micropipette 500 - 5000 µl
- VITLAB® micropipette 1000 - 10000 µl
- Tip-Box 50 - 1000 µl
- Tip-Box 0.5 - 5 ml
- Tip-Box 1 - 10 ml
- Rack mount (3x)

Cat. No.: 33333

# Pipetting

## Accessories for VITLAB® micropipettes

With the practical rack mount and freely rotatable bench-top stand, VITLAB® micropipettes can be stored safely and ready to use.

Description	PU	Cat. No.
Wall mount for 1 pipette	1	1672000
Bench-top stand for 6 singlechannel or 6 multichannel instruments	1	1672002
Filter for pipette, 5 ml	25	1672010
Filter for pipette, 10 ml	25	1672012
Silicone grease for pipettes, up to 1000 µl	1	1672015
Silicone grease for pipettes 5 ml / 10 ml and multichannel pipettes	1	1672016
Fluorostatic grease for multichannel pipettes	1	1670050



## Reagent reservoir, non-sterile, PP



Transparent, with lid to guard against contamination and spilling out of contents during movement. Optimally suited for working with multichannel pipettes. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	PU	Cat. No.
60	10	319099



## Pipette tip selection guide

Which pipette tip will fit my VITLAB® micropipette?

Nominal volume VITLAB® micropipettes							Nominal volume VITLAB® micropipette -8/-12				Tip volume
10 µl	20 µl	100 µl	200 µl	1000 µl	5 ml	10 ml	50 µl	100 µl	200 µl	300 µl	
◆											0.5 - 20 µl
	◆	◆	◆				◆	◆	◆		2 - 200 µl
		◆	◆				◆	◆	◆	◆	5 - 300 µl
				◆							50 - 1000 µl
					◆						0.5 - 5 ml
						◆					1 - 10 ml





## VITLAB<sup>®</sup> pipette tips

VITLAB<sup>®</sup> pipette tips are made from high-quality polypropylene and are autoclavable at 121 °C (2 bar) according to DIN EN 285. The raw material used is free from additives such as DiHEMA (di(2-hydroxyethyl)methyl-dodecyl-ammonium) and oleamide (9-octadecenamide) that often cause interference, particularly in biological labs. All palletized pipette tips up to 1000 µl are **free of DNA (< 40 fg), RNase (< 8.6 fg), endotoxins (< 1 pg) and ATP (< 1 fg)**. The pipette tips are **CE marked according to the IVD guideline 98/79 EC** and optimally suited for VITLAB<sup>®</sup> micropipettes.

Furthermore, the tips are compatible with most pipette models from BRAND, GILSON<sup>®</sup>, Thermo Fisher Scientific FINNPIPETTE<sup>®</sup>, Eppendorf<sup>®</sup> and sartorius<sup>®</sup> Biohit<sup>®</sup>. The 5 ml tip is only tested for VITLAB, BRAND and Thermo Fisher Scientific FINNPIPETTE<sup>®</sup>. The 10 ml tip is only tested for VITLAB, BRAND and Eppendorf<sup>®</sup>. Note: Pipette shafts are subject to modification and should be checked before use. The fit depends on the manufacturer, pipette type, serial number, and date of manufacture, among other things.

## Packaging variations

VITLAB<sup>®</sup> pipette tips are available in the variations palletized in the Tip-Box and packed in bags. Additionally, empty Tip-Boxes for self-filling are available. Tip-Boxes up to 1000 µl are stackable and their format conforms to the common 96 (8x12) unit format.



### Resealable bags

All tips up to 1000 µl are produced under cleanroom conditions, automatically shrink-wrapped in reclosable bags and packaged in cartons. The article number, volume range and lot number of the tips are printed on every bag.



### Tip-Box (up to 1000 µl)

PP box with functional hinged and snap-on lid. For all volume ranges up to 1000 µl in practical 8x12 format. Stackable and autoclavable at 121 °C according to DIN EN 285.



### Tip-Box 5/10 ml

PP box with fitted lid. Filled with 5 ml (28 pcs.) or 10 ml (18 pcs.) tips. The box is autoclavable at 121 °C according to DIN EN 285.



# Pipetting

## Pipette tips, 0.5 – 20 µl



PP, non-sterile with graduation at 2 and 10 µl. Length: 46 mm. Slim tip for contact-free pipetting into microtiter plates. Tip-Box with gray mounting plate for easy identification; palletized tips are colourless.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 1000 tips	2000	148894
Bag, Maxi	10 bags with 1000 tips	10000	155494
Tip-Box, filled	Box with 96 tips on gray mounting plate	5	149794
Tip-Box, empty	Box with gray mounting plate, without tips	1	155400



## Pipette tips, 2 – 200 µl



PP, non-sterile with graduation at 20 and 100 µl. Length: 50 mm. Tip-Box with yellow mounting plate for easy identification; palletized tips are colourless. Tips in bags are coloured yellow.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 1000 tips	1000	148994
Bag, Maxi	10 bags with with 1000 tips	10000	155694
Tip-Box, filled	Box with 96 tips on yellow mounting plate	5	149994
Tip-Box, empty	Box with yellow mounting plate, without tips	1	155600




## Pipette tips, 5 - 300 µl



PP, non-sterile with graduation at 50, 100 and 300 µl. Length: 53 mm. Also suitable for pipettes with yellow colour-code (see selection guide p. 25). Tip-Box with green mounting plate for easy identification; palletized tips are colourless. Tips in bags are also colourless.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 1000 tips	1000	149094
Bag, Maxi	10 bags with 1000 tips	10000	155894
Tip-Box, filled	Box with 96 tips on green mounting plate	5	150094
Tip-Box, empty	Box with green mounting plate, without tips	1	155800



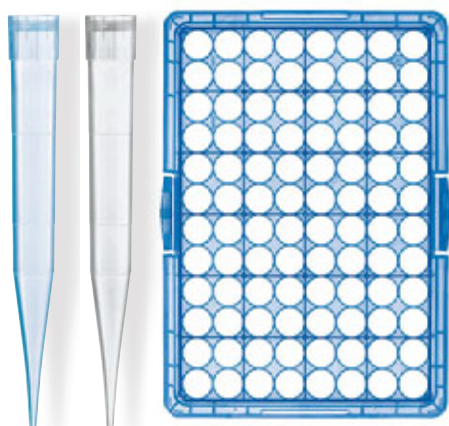

## Pipette tips, 50 - 1000 µl



PP, non-sterile with graduation at 250, 500 and 1000 µl. Length: 70 mm. Tip-Box with blue mounting plate; palletized tips are colourless. Tips in bags are coloured blue.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 500 tips	1000	149194
Bag, Maxi	10 bags with 500 tips	5000	155994
Tip-Box, filled	Box with 96 tips on blue mounting plate	5	150194
Tip-Box, empty	Box with blue mounting plate, without tips	1	155900



## Pipette tips, 0.5 - 5 ml



PP, non-sterile. Length: 160 mm. Diameter: approx. 9.6 mm. Slim shape for pipetting into narrow vessels such as measuring flasks with NS 12/21.

Variation	Packaging	PU	Cat. No.
Bag, Standard	1 bag with 200 tips	200	146294
Tip-Box, filled	Box with 28 tips	1	150294



## Pipette tips, 1 -10 ml



PP, non-sterile. Length: 156.5 mm. Diameter: approx. 15 mm.

Variation	Packaging	PU	Cat. No.
Bag, Standard	2 bags with 100 tips	200	146494
Tip-Box, filled	Box with 18 tips	1	150394

# Perfection in Liquid Handling

RAPID AND ACCURATE TITRATION



## VITLAB® continuous E/RS



The VITLAB® continuous bottle-top burette (Figure 1) enables continuous titration, which leads to fast, convenient and accurate results. The angled display shows 4-position titration volume in large, easily read numbers (Figure 2), which simplifies operation. Turning the two hand wheels supplies the titration medium in a **continuous and pulse-free** manner via the specially developed double-piston pump (Figure 3). Filling procedures are not necessary. This innovative technology increases safety; its compact design and low centre of gravity reduce risk of falling over, especially with smaller bottles. The height and length of the discharge tube can be adjusted, making it possible to work safely with both short and tall bottles. The innovative recirculation system (Figure 4) **prevents the loss of valuable reagent** and reduces the risk of splashes. With its simple-to-use calibration function, VITLAB® continuous fulfils the corresponding requirements for test equipment monitoring without instrument downtime. Margins of error are under those specified in the DIN EN ISO 8655-3 standard, even for partial volumes. VITLAB® continuous is DE-M marked. Also available with DAkkS calibration certificate (at additional cost).

Included in delivery:

VITLAB® continuous E/RS (GL 45 thread), 3 PP thread adapters (GL 32, GL 38 and S 40), telescopic filling tube (200 - 350 mm), telescopic discharge tube (140 - 220 mm), two microbatteries 1.5 V (LR 03/AAA), quality certificate and operating manual.



Type	Nominal volume ml	A* ≤ ± %	CV* ≤ %	PU	Cat. No.
E	25	0.2 at 25 ml	0.1 at 25 ml	1	1620506
RS	50	0.2 at 50 ml	0.1 at 50 ml	1	1620507

\* Error tolerance conforming to DIN EN ISO 8655-3, related to the nominal (maximum) volume marked on the device where the device, environment and distilled H<sub>2</sub>O are at the same temperature (20 °C). Checks are done in accordance with DIN EN ISO 8655-6 with the device filled to capacity and with uniform and jolt-free dosing. DE-M marked.



The VITLAB® continuous E/RS bottle-top burette can be used for the following titrants up to a concentration of 1 mol/L:

Acetic acid	Potassium hydroxide
Ammonium iron (II) sulphate solution	Potassium iodate solution
Ammonium thiocyanate solution	Potassium permanganate solution
Barium chloride solution	Potassium thiocyanate solution
Bromide bromate solution	Silver nitrate solution
Cerium (IV) sulphate solution	Sodium arsenite solution
EDTA solution	Sodium carbonate solution
Hydrochloric acid	Sodium chloride solution
Iron (II) sulphate solution	Sodium hydroxide
Nitric acid	Sodium nitrite solution
Oxalic acid solution	Sodium thiosulphate solution
Perchloric acid	Sulphuric acid
Potassium bromate solution	Tetra-n-butylammonium hydroxide solution
Potassium bromide / bromate solution	Zinc sulphate solution
Potassium dichromate solution	

The recommendations in this table have been carefully tested and reflect the most current information available. Always follow the instruction manual for the instrument as well as the reagent manufacturer's specifications. Should you require information on chemicals not listed, please do not hesitate to contact us. As at 03/17.





# Titration

## Adapter for VITLAB® continuous E/RS

For secure screwing of the burettes onto reagent bottles with an NS neck, GL screw threading or an S buttress thread.

Description	External thread	Bottle neck threads	PU	Cat. No.
NS-adapter, PP	GL 32	NS 19/26	1	1670066
NS-adapter, PP	GL 32	NS 24/29	1	1670067
NS-adapter, PP	GL 32	NS 29/32	1	1670068
Thread adapter, PP	GL 32	GL 28	1	1670155
Thread adapter, PP	GL 38	GL 32	1	1670085
Thread adapter, PP	GL 45	GL 32	1	1670180
Thread adapter, PP	GL 45	GL 38	1	1670110
Thread adapter, PP	GL 45	S 40	1	1670120
Thread adapter, ETFE	GL 32	GL 28	1	1670080
Thread adapter, PTFE	GL 38	GL 32	1	1670095
Thread adapter, ETFE	GL 45	GL 32	1	1670100
Thread adapter, ETFE	GL 45	GL 38	1	1670115
Thread adapter, PTFE	GL 45	S 40	1	1670125



The suitable plastic tripod can be found on page 15.

## Drying tube for VITLAB® continuous E/RS

PP, transparent, unfilled. Can be connected directly to the burette.

Description	PU	Cat. No.
Drying tube, PP, unfilled	1	1671095



## Telescopic filling tube for VITLAB® continuous E/RS

For the filling of titration medium from bottles of different heights.

Description	Length mm	PU	Cat. No.
Telescopic filling tube, FEP, ETFE, PTFE	200 - 350	1	1671085



## Bottles for VITLAB® continuous E/RS

Threaded brown glass (soda lime glass) bottles with an ethylene acrylate coating.

Volume ml	Thread GL	Shape	PU	Cat. No.
1000	45	square	1	1671500
2500	45	round	1	1671510






## VITLAB® Dr. Schilling burettes

Burettes made of borosilicate glass 3.3, tolerances according to DIN ISO 384 Class B, with high-contrast black markings. Calibrated to deliver 'Ex'. Automatic zero setting. The burette stopcock turns easily and enables fine titration. The holding device for the riser pipe serves as additional shock-proofing.

The patented VITLAB® symbiotic (DE 10 2005 034 963) offers in addition to the impact protection a thermally stable plastic coating of the glass burette tube. This provides additional breaking resistance and acts as a splinter protection.

Materials: burette of borosilicate glass 3.3, PP filling tube, PMP/PTFE burette stopcock, and PE-LD reservoir bottle.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Bottle ml	PU	Cat. No.
VITLAB® symbiotic, with Schellbach stripes (blue/white)						
25	0.05	0.05	900	1000	1	106599
50	0.10	0.10	900	1000	1	106699
Burette with Schellbach stripes (blue/white), without plastic-coating						
25	0.05	0.05	900	1000	1	106399
50	0.10	0.10	900	1000	1	106499
Burette made of brown glass, without Schellbach stripes, without plastic-coating						
25	0.05	0.05	900	1000	1	106799
50	0.10	0.10	900	1000	1	106899

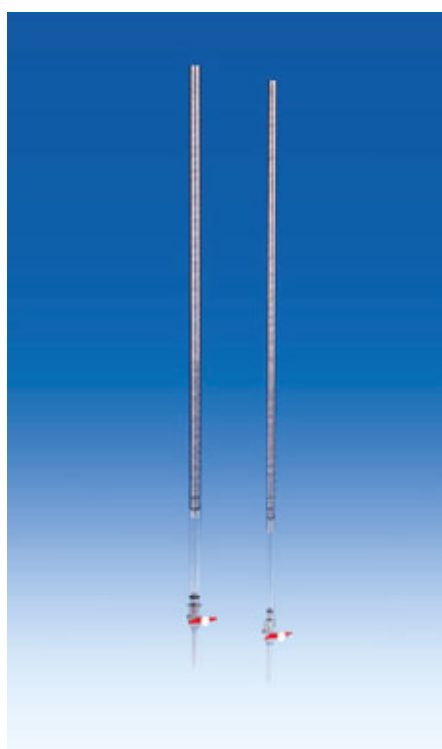

## Burettes, borosilicate glass 3.3

Plastic-coated burette made of borosilicate glass 3.3, tolerances corresponding to DIN ISO 384, Class B. With Schellbach stripes (blue/white) and high-contrast black marking. Calibrated to deliver 'Ex'. The burette stopcock turns easily and enables fine titration. The temperature-stable plastic coating on the tube provides splinter protection.

Materials: Burette of borosilicate glass 3.3, with PMP/PTFE burette stopcock.

Volume ml	Tolerance ± ml	Graduation ml	Length mm	PU	Cat. No.
25	0.05	0.05	800	2	105599
50	0.10	0.10	800	2	105699



# Titration

## Burette stopcocks, PMP/PTFE

Stopcocks made of PMP. Plugs of PTFE with polished surfaces, turn easily. Insert with two seals.

Cat. No. 105799: For 25 ml tubes with an inner diameter of  $7.75 \pm 0.1$  mm.

Cat. No. 105899: For 50 ml tubes with an inner diameter of  $11.5 \pm 0.1$  mm.

For burettes ml	Tip inner Ø mm	PU	Cat. No.
25	1.25	5	105799
50	1.25	5	105899



## Burette clamps, PP

Practical holder for anchoring burettes vertically on the support stand. The volume scale remains clearly readable.

Burette clamps with slip-resistant rubber-coated tips and springs made of stainless steel.

With stand clamps for securing to rods of  $\varnothing$  8-14 mm.

Type	PU	Cat. No.
For 1 burette	5	80139
For 2 burettes	5	80140



# Calibration certificates

---

For all volumetric instruments that are subject to test equipment monitoring, a written documentation about the regularly calibration resp. volume control is necessary. The documentation should contain the values for accuracy and coefficient of variation as well as the testing procedure and test frequency. A distinction is made between:

- Quality certificates (factory calibration report)
- Official calibration certificates (Bureau of standards, DAkkS)

## Quality certificates

The VITLAB quality certificate is a factory calibration report on the basis of the quality assurance system according to DIN EN ISO 9001. Quality certificates are available as a batch or individual certificate. Devices from one production batch have the same lot number as the quality certificate. The certificate records for the specific batch the mean value, standard deviation and day of issue. In the case of an individual certificate\*, the volumetric instrument and the certificate bear an individual serial number in addition to the lot number. The certificate records besides the day of issue also the measured volume and the measurement uncertainty.

## DAkkS calibration certificate

The DAkkS calibration certificate\* documents officially the traceability of measuring results to national and international standards as required by the standards DIN EN ISO 9001 and DIN EN ISO / IEC 17025 for the monitoring of measuring instruments. A major difference between factory calibration services and DAkkS laboratories is the accurate determination of the respective uncertainty of measurement guaranteed by the accredited laboratory and supervised by the DAkkS. DAkkS calibration certificates are appropriate in uses in which calibrations of an accredited laboratory are requested, where high level calibrations are demanded and for calibration of reference standards and instruments for comparative measurements.

## Calibration service

VITLAB offers a repair, maintenance and calibration service (incl. DAkkS calibration) for all Liquid Handling devices made by VITLAB. The calibration laboratory accredited by the „Deutsche Akkreditierungsstelle GmbH“ (DAkkS) is authorized to issue DAkkS Calibration certificates for the following instruments: Liquid Handling products like VITLAB piston-operated pipettes and burettes, VITLAB dispensers and VITLAB volumetric plastic labware.

\* Available at additional cost

# Competence in Volume Measurement

EXCELLENCE IN MEASUREMENT ACCURACY





# The very highest volumetric instr

Volume measurement is a routine laboratory operation. Therefore, volumetric instruments such as volumetric flasks, measuring cylinders and pipettes are standard equipment in any analytical laboratory.

The importance of the standard of measurement accuracy in your routine laboratory operations cannot be overstated. VITLAB has decades of experience in the development and production of laboratory products which are used to measure volumes. VITLAB is the first manufacturer to produce Class A measuring cylinders from PMP that are certified compliant according to DIN 12681.

All Class A PMP volumetric flasks are optionally available in transparent or UV-absorbing variations for light-sensitive substances.

# High precision instruments

## Calibration

**Type "Ex":** The delivered quantity of liquid corresponds to the volume printed on the instrument (pipettes and burettes).

**Type "In":** The contained quantity of liquid corresponds to the volume printed on the instrument (volumetric flasks and measuring cylinders).

VITLAB calibrates each individual volumetric flask "to contain" (In) at a reference temperature of 20 °C. The hydrophobic characteristics of the materials in plastic volumetric instruments lead to the measured volume being the same as the delivered quantity ("In" = "Ex") for aqueous solutions.

## Accuracy classes

**Class A:** The volume tolerances lie within the limits specified by DIN and ISO.

**Class B:** The volume tolerances are twice the error limits for Class A specified by DIN and ISO. Detailed explanations on "accuracy in volume measurement" are available in the chapter on "General and Technical Information".

## Certificate of conformity

The DE-M marking is VITLAB's guarantee that the respective products comply with the German Measurement and Calibration Regulation. The special manufacturing process developed by VITLAB, and the proven VITLAB quality management system, ensure compliance with the volume tolerances specified by the standards.





## Volumetric flasks, PFA, Class A, with screw cap, PFA



Highly transparent.

Ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

The PFA screw cap guards against contamination.

Outstanding chemical resistance, can be used with strong oxidants, highly concentrated acids and alkalis, hydrocarbons, and ketones.

With laser-engraved lot number and batch certificate. Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve the ring mark, do not clean at temperatures exceeding 60 °C.

Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

The advantages of PFA:

- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability, suitable for volumetric instruments
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.04	90	18	1	107097
25	0.04	115	18	1	107197
50	0.06	150	18	1	107297
100	0.10	180	18	1	107397
250	0.15	235	25	1	107497
500	0.25	270	25	1	107597

\* Height without screw cap

Replacement screw caps  
can be found on page 105.

### Compare: VITLAB® volumetric flasks ...

- ... have a circular, precisely calibrated ring mark with which the meniscus can be read accurately from any position
- ... have a straight neck for precise volume measurement
- ... have a specially formed bottom for superior stability

... are MADE IN GERMANY



# Volume measurement

## VITLAB® opaque volumetric flasks, PMP, Class A with NS stoppers, PP



UV-absorbing, highly transparent. For storage of light-sensitive substances.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.04	90	10/19	2	670950
25	0.04	115	10/19	2	671950
50	0.06	150	12/21	2	672950
100	0.10	180	14/23	2	673950
250	0.15	235	19/26	2	674950
500	0.25	270	19/26	2	675950
1000	0.40	310	24/29	1	676950

\* Height without stopper



Replacement stoppers  
can be found on page 112.

**VITLAB® opaque replaces brown glass**  
and is...

- ... substantially lighter in weight
- ... practically unbreakable
- ... practically impermeable in the UV region
- ... comparable to a light protection factor of 20

## VITLAB® opaque volumetric flasks, PMP, Class A, with coloured screw caps, PP



UV-absorbing, highly transparent. For storage of light-sensitive substances.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.04	90	18	2	670040
25	0.04	115	18	2	671040
50	0.06	150	18	2	672040
100	0.10	180	18	2	673040
250	0.15	235	25	2	674040
500	0.25	270	25	2	675040
1000	0.40	310	32	1	676040

\* Height without screw cap



Replacement screw caps  
can be found on page 107.

More information on VITLAB® opak can be found on page 132.



## Volumetric flasks, PMP, Class A with NS stoppers, PP



Highly transparent.

With ring mark individually calibrated to 'In'.

Class A tolerances according to DIN EN ISO 1042.

With printed lot number and batch certificate.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.04	90	10/19	6	67704
25	0.04	115	10/19	6	67104
50	0.06	150	12/21	6	67204
100	0.10	180	14/23	6	67304
250	0.15	235	19/26	5	67404
500	0.25	270	19/26	4	67504
1000	0.40	310	24/29	3	67604

\* Height without stopper

Replacement stoppers  
can be found on page 112.



## Volumetric flasks, PMP, Class B with NS stoppers, PP



Highly transparent.

With ring mark individually calibrated to 'In'.

Class B tolerances according to DIN EN ISO 1042.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.08	90	10/19	6	67795
25	0.08	115	10/19	6	67195
50	0.12	150	12/21	6	67295
100	0.20	180	14/23	6	67395
250	0.30	235	19/26	5	67495
500	0.50	270	19/26	4	67595
1000	0.80	310	24/29	3	67695

\* Height without stopper

Replacement stoppers  
can be found on page 112.

# Volume measurement

## Volumetric flasks, PMP, Class B with screw caps, PP



Highly transparent.

With ring mark individually calibrated to 'In'.

Class B tolerances according to DIN EN ISO 1042.

Thermal stress up to 121 °C (autoclaving) does not permanently exceed the tolerance limit.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.08	90	18	6	677895
25	0.08	115	18	6	671895
50	0.12	150	18	6	672895
100	0.20	180	18	6	673895
250	0.30	235	25	5	674895
500	0.50	270	25	4	675895
1000	0.80	310	32	3	676895

\* Height without screw cap



→ Replacement screw caps can be found on page 107. →



## Volumetric flasks, PP, Class B with NS stoppers, PP



Highly transparent.  
With ring mark individually calibrated to 'In'.  
Class B tolerances according to DIN EN ISO 1042.  
Thermal stress up to 60 °C does not permanently exceed the tolerance limits.  
To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Neck NS	PU	Cat. No.
10	0.08	90	10/19	6	677941
25	0.08	115	10/19	6	671941
50	0.12	150	12/21	6	672941
100	0.20	180	14/23	6	673941
250	0.30	235	19/26	5	674941
500	0.50	270	19/26	4	675941
1000	0.80	310	24/29	3	676941

\* Height without stopper

Replacement stoppers  
can be found on page 112.



## Volumetric flasks, PP, Class B, with screw cap, PP



Highly transparent.  
With ring mark individually calibrated to 'In'.  
Class B tolerances according to DIN EN ISO 1042.  
Thermal stress up to 60 °C does not permanently exceed the tolerance limits.  
To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Tolerance ± ml	Height* mm	Thread GL	PU	Cat. No.
10	0.08	90	18	6	677891
25	0.08	115	18	6	671891
50	0.12	150	18	6	672891
100	0.20	180	18	6	673891
250	0.30	235	25	5	674891
500	0.50	270	25	4	675891
1000	0.80	310	32	3	676891

\* Height without screw cap

Replacement screw caps  
can be found on page 107.

# Volume measurement

## Graduated cylinders, PMP, Class A, tall form, red printed graduations



Highly transparent. DE-M marked.

With red printed graduations and ring marks at the primary scale points, calibrated 'In'.

The lot certificate supplied bears the batch number and the actual nominal value ascertained under the test conditions. The resulting deviations from the nominal value fall well under the allowed tolerances of Class A according to DIN 12681 and ISO 6706.

With printed batch number and year of production. Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

Hexagonal base with bottom studs provides high stability. To preserve markings, do not clean at temperatures exceeding 60 °C. Thus, conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving we recommend the design with molded graduations (Cat.-No. 64604 – 65304).

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.10	0.20	145	15	2	64614
25	0.25	0.50	170	22	2	64714
50	0.50	1.00	200	27	2	64814
100	0.50	1.00	250	33	2	64914
250	1.00	2.00	315	44	2	65014
500	2.50	5.00	360	58	1	65114
1000	5.00	10.00	440	69	1	65214
2000	10.00	20.00	535	97	1	65414



## Graduated cylinders, PMP, Class A, tall form, molded graduations



Highly transparent. DE-M marked.

With molded graduations and ring marks at the primary scale points, calibrated 'In'.

The lot certificate supplied bears the batch number and the actual nominal value ascertained under the test conditions. The resulting deviations from the nominal value fall well under the allowed tolerances of Class A according to DIN 12681 and ISO 6706. With the laser engraved batch number and the year of manufacture. Also available with DAkkS calibration certificate or individual quality certificate (at additional cost).

Hexagonal base with bottom studs provides high stability. Thermal stress up to 121 °C (autoclaving) does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.10	0.20	145	15	2	64604
25	0.25	0.50	170	22	2	64704
50	0.50	1.00	200	27	2	64804
100	0.50	1.00	250	33	2	64904
250	1.00	2.00	315	44	2	65004
500	2.50	5.00	360	58	1	65104
1000	5.00	10.00	440	69	1	65204
2000	10.00	20.00	482	97	1	65304





## Graduated cylinders, PP, Class B, tall form, with molded blue graduations



Highly transparent.

With easily readable, molded, embossed blue graduations and ring marks at the primary scale points. Calibrated 'In'. Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded. To preserve markings, do not clean at temperatures exceeding 60 °C.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.20	0.20	145	15	12	646081
25	0.50	0.50	170	22	12	647081
50	1.00	1.00	200	27	12	648081
100	1.00	1.00	250	33	12	649081
250	2.00	2.00	315	44	6	650081
500	5.00	5.00	360	58	6	651081
1000	10.00	10.00	440	69	6	652081
2000	20.00	20.00	482	97	3	653081



## Graduated cylinders, PP, Class B tall form, with molded graduations



Highly transparent.

With molded graduations and ring marks at the primary scale points, calibrated 'In'. Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
10	0.20	0.20	145	15	12	646941
25	0.50	0.50	170	22	12	647941
50	1.00	1.00	200	27	12	648941
100	1.00	1.00	250	33	12	649941
250	2.00	2.00	315	44	6	650941
500	5.00	5.00	360	58	6	651941
1000	10.00	10.00	440	69	6	652941
2000	20.00	20.00	482	97	3	653941



# Volume measurement

## Graduated cylinders, SAN, Class B tall form, with molded graduations



Crystal clear.

With molded graduations and ring marks at the primary scale points, calibrated 'In'.

Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 60 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
50	1.00	1.00	199	28	12	64891
100	1.00	1.00	260	34	12	64991
250	2.00	2.00	315	47	6	65091
500	5.00	5.00	350	61	6	65191
1000	10.00	10.00	415	76	6	65291



## Graduated cylinders, PP, Class B short form, with molded graduations



Highly transparent.

With molded graduations, calibrated 'In'.

Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
25	0.50	0.50	122	22	12	640941
50	1.00	1.00	142	27	12	641941
100	2.00	2.00	163	37	12	642941
250	5.00	5.00	192	51	6	643941
500	10.00	10.00	218	67	6	644941
1000	20.00	20.00	285	78	6	645941





## Graduated cylinders, SAN, Class B, short form, with molded graduations



Crystal clear.

With molded graduations, calibrated 'In'.

Thermal stress up to 60 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Tolerance ± ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
25	0.50	0.50	122	22	12	64091
50	1.00	1.00	142	27	12	64191
100	2.00	2.00	163	37	12	64291
250	5.00	5.00	192	51	6	64391
500	10.00	10.00	218	67	6	64491
1000	20.00	20.00	285	78	6	64591

Compare: VITLAB® graduated cylinders...

... have guaranteed seamless interiors, which mean the analysis is unaffected by residues and carryover

... have precise calibration ring marks at the primary scale points, with which the meniscus can be read accurately

... a sturdy, even stand for precise volume measurement

... are MADE IN GERMANY



## Hydrometer cylinder, PP

Highly transparent, with spout and overflow vessel. For density measurements using a hydrometer. Hydrometer can be read through the overflow vessel with a completely filled cylinder.

With molded graduations and ring marks at the primary scale points, calibrated 'In'.

Class B tolerances according to DIN 12681 / ISO 6706.

Hexagonal base with bottom studs provides high stability. Thermal stress up to 80 °C does not cause tolerance limits to be permanently exceeded.

Volume ml	Graduation ml	Height mm	Ø mm	PU	Cat. No.
500	5.00	351	73	1	760941

# Volume measurement

## Bulb pipettes, PP, Class B

Calibrated to deliver 'Ex'.

Highly transparent. With high-contrast, blue markings.

Break-resistant.

High chemical resistance.

Exposure to temperatures above 60 °C can lead to volume changes.

Recommended cleaning with mild alkaline detergents up to 60 °C.

Volume ml	Tolerance ± ml	Length mm	PU	Cat. No.
1	0.02	300	12	164094
2	0.02	300	12	164194
5	0.03	300	6	164294
10	0.04	440	6	164394
25	0.05	450	6	164494
50	0.10	460	6	164594



## Graduated pipettes, PP, Class B

Calibrated to deliver 'Ex'.

Highly transparent. With high-contrast, blue markings.

Break-resistant.

High chemical resistance.


Outer diameter of suction tube: max. 8 mm.

Exposure to temperatures above 60 °C can lead to volume changes.

Recommended cleaning with mild alkaline detergents up to 60 °C.

Volume ml	Tolerance ± ml	Graduation ml	Length mm	PU	Cat. No.
1	0.02	0.1	300	12	163094
2	0.02	0.1	300	12	163194
5	0.05	0.1	330	12	163294
10*	0.10	0.1	330	12	163394
10	0.10	0.1	320	12	163594

\* Suction tube outer diameter: 10 mm

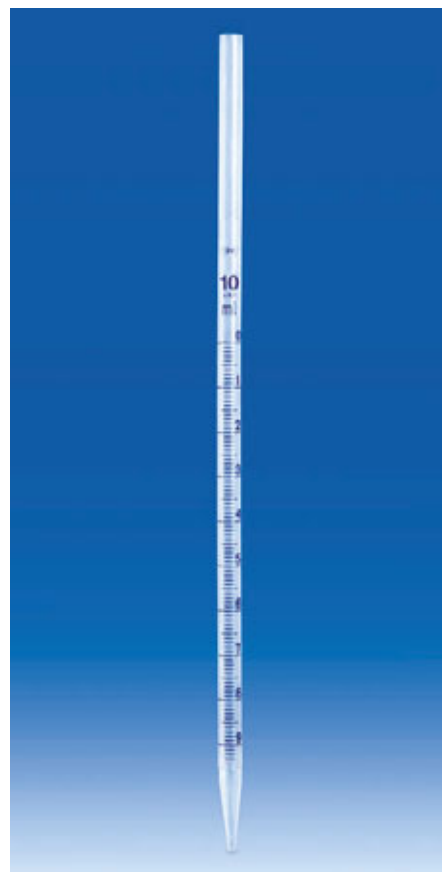



## Disposable pipettes, PS, sterile



Crystal clear, graduated, individual sterile packaging, pyrogen-free. Identified by bar-code. With cotton-wool filter.

Volume ml	Graduation ml	Length mm	PU	Cat. No.
1	0.01	272	25	160110
2	0.01	272	25	160210
5	0.10	320	25	160510
10	0.10	320	25	161010
25	0.20	345	10	162510



## Disposable pipettes, PS, non-sterile

Crystal clear, graduated, non-sterile. Identified by bar-code. With cotton-wool filter.

Volume ml	Graduation ml	Length mm	PU	Cat. No.
1	0.01	272	10	160119
2	0.01	272	10	160219
5	0.10	320	10	160519
10	0.10	320	10	161019

→ Pipette helpers  
can be found on pages 49 - 51. →

# Volume measurement

## VITLAB pipeo®



For all pipettes from 0.1 to 200 ml.

With the VITLAB pipeo® pipette controller, pipette handling is simple and comfortable. The ergonomic handle - **very light weight** at about 190 grams - and excellent balance all contribute to ease of operation. The speed can be adjusted easily, continuously and exactly with one hand using two buttons. A 50 ml pipette can be filled comfortably in less than ten seconds. The liquid release can be done either by gravity delivery when calibrated 'Ex' (to deliver), or in blow out mode using the battery-operated motor.

Pipettes are held securely and tightly in the exchangeable adapter. Liquid vapours are purged directly to protect the instrument.

One full charge of the nickel-metal hydride battery allows 8 hours of non-stop pipetting. The charge level of the recyclable battery is shown by the LED indicator. Defective batteries are easily replaced. To avoid surprises, the LED light changes from green to red two hours before the battery must be recharged. **The VITLAB pipeo® can still be operated while the battery is being recharged.**



Included in delivery:

VITLAB pipeo®, battery charger (100 - 240 V, 50/60 Hz), four plug adapters (EU, UK, US/J, AUS), battery, battery compartment cover, two replacement 0.2 µm membrane filters and operating manual.

Description	PU	Cat. No.
pipeo®	1	1631500



## VITLAB maneus®



The VITLAB maneus® Pipette Helper enables both left- and right-handers to operate all current volumetric and graduated pipettes from 0.1 to 200 ml easily and fatigue-free. Its safe and easy handling allows even inexperienced users **to adjust the meniscus precisely**.

With the design, unscrewing the adapter enables easy replacement of the hydrophobic membrane filter, which **protects the instrument against fluid penetration**.

The valve system is optimised so that liquids can be drawn up simply, without exerting pressure. The highly sensitive filling and discharge of liquids are controlled gently by the pipetting knob. Thus, the suction element provides rapid filling of the pipette (capacity: 50 ml in less than 10 seconds). The discharge bellows are used for the emptying (blow-out) of the pipette. The specially moulded intake cone ensures secure seating for all normal bulb and graduated pipettes (0.1 to 200 ml).

The VITLAB maneus® is simple to dismantle, easy to clean, and completely autoclavable at 121 °C (2 bar) according to DIN EN 285.

Included in delivery: VITLAB maneus®, replacement 3 µm membrane filter und operating manual.

Description	PU	Cat. No.
maneus®	1	1630500



## Accessories for VITLAB pipeo® & maneus®

Description	PU	Cat. No.
Membrane filter, 0.2 µm, sterile, VITLAB pipeo®	1	1670647
Membrane filter, 0.2 µm, non-sterile, VITLAB pipeo®	10	1670648
Membrane filter, 3 µm, non-sterile, VITLAB pipeo®, VITLAB maneus®	10	1670650
Wall rack, VITLAB pipeo®	1	1670660



# Volume measurement

## Pipette fillers, NR

Classic accessory for pipetting with volumetric or measuring pipettes. With 3 valves.  
Valve A: Air release, Valve S: Liquid filling, Valve E: Liquid dispensing.

Type	PU	Cat. No.
Universal model, for pipettes up to 10 ml	1	104099
Universal model, for pipettes up to 100 ml	1	104199



## Pipette fillers

For pipetting liquids, fit all glass and plastic pipettes. Slow rotation of the actuator-wheels draws liquid into the pipette. Pressing the air bleed valve automatically empties the pipette without returning the piston.

For pipettes ml	Colour	PU	Cat. No.
2	Blue	1	324594
10	Green	1	324694
25	Red	1	324794





## Pipette stand, PP

Upper portion with 94 bore holes of different diameters for secure placement of volumetric and measuring pipettes of any size.

The stable base has a rotatable, ribbed base plate in which the pipette tips can be gently seated.

The racks are supplied unassembled, and can easily be assembled according to the accompanying assembly instructions.

Ø mm	Height mm	PU	Cat. No.
230	470	2	79194



## Pipette tray, PVC

For pipettes of various sizes. Can accommodate 7 pipettes lengthwise (with max. 20 mm diameter) or 16 pipettes sideways (with a diameter of max. 10 mm). Pipettes can easily be placed in and taken out from the troughs in the tray, even with gloves.

L x W x H mm	PU	Cat. No.
283 x 216 x 40	1	80996



## Pipette tray for drawers, PVC

Suitable for drawers, divided lengthwise into 4 compartments.

L x W x H mm	PU	Cat. No.
426 x 300 x 30	1	80252

# Volume measurement

## Pipette washer, PE-HD

For simple and basic cleaning of pipettes. With discharge siphon for an automatic water exchange.

The complete washing system includes the pipette washer, pipette jar (for pre-cleaning) and pipette basket (for dipping pipettes into the pipette washer or pipette jar). Pipette jars and pipette baskets need to be ordered separately.

Suitable for the use with pipette baskets (cat. nos. 80219 and 80222).

Ø mm	Height mm	Effective length mm	PU	Cat. No.
170	734	600	1	80217
170	990	840	1	80215



## Pipette jars, PE-HD

For pre-cleaning pipettes in detergent solutions.

Suitable for the use with pipette baskets (cat. nos. 80219 and 80222).

Ø mm	Height mm	PU	Cat. No.
125	250	1	80223
162	503	1	80221
162	650	1	80218



## Pipette baskets, PE-HD

For dipping pipettes into the pipette jar or pipette-washer and for transferring pipettes.

Basket height 300 mm.

With the extension piece, the total height of the pipette basket (cat. no. 80219) increases from 650 to 870 mm.

Description	Ø mm	Overall height mm	PU	Cat. No.
Pipette basket	145	648	1	80219
Pipette basket	145	497	1	80222
Extension piece for the handle (pipette basket 80219)			2	81219





# Competence in Plastic Labware

MEASURING AND TRANSFERRING



**VITLAB**   
Competence in Labware



## Graduated beakers, PP, molded blue graduations



Highly transparent. With easily readable, molded, embossed blue graduations, and stable, easy-grip handle. To preserve markings, do not clean at temperatures exceeding 60 °C. Conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving, we recommend the design with molded graduations (cat. nos. 440941 - 447941).

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
50	2	70	40	24	446081
100	2	80	50	24	447081
250	5	120	74	12	440081
500	10	140	92	12	441081
1000	10	181	117	6	442081
2000	20	213	152	6	443081
3000	50	242	172	6	444081
5000	50	270	204	6	445081



## Graduated beakers, PP, molded graduations



Highly transparent. With molded graduations and stable, easy-grip handle. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
50	2	70	40	24	446941
100	2	80	50	24	447941
250	5	120	74	12	440941
500	10	140	92	12	441941
1000	10	181	117	6	442941
2000	20	213	152	6	443941
3000	50	242	172	6	444941
5000	50	270	204	6	445941



# Measuring and transferring

## Graduated beakers, PP, nesting



Highly transparent. With stable handle and easily readable, printed black graduations on both sides. Therefore, the volume is equally visible for left- and right handers. With recess in the handle for better water drainage in the dishwasher. To preserve markings, cleaning at no higher than 60 °C is recommended. For autoclaving we recommend the design with molded graduations (cat. nos. 440941 - 447941).



Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
250	5	115	75	12	480941
500	10	140	100	12	481941
1000	10	167	125	12	482941
2000	20	212	148	12	483941
3000	50	242	170	12	484941

## Graduated beakers, PP, nesting, coloured



Graduated beakers in four different colours. Transparent, with stable handle and easily readable, printed graduations on both sides. Therefore, the volume is equally visible for left- and right handers. With recess in the handle for better water drainage in the dishwasher. To preserve markings, cleaning at no higher than 60 °C is recommended. For autoclaving we recommend the design with molded graduations (cat. nos. 440941 - 447941).



Volume ml	Colour	Divisions ml	Height mm	Ø mm	PU	Cat. No.
500	blue	10	140	100	12	481942
500	yellow	10	140	100	12	481943
500	red	10	140	100	12	481944
500	green	10	140	100	12	481945
500	Set: blue, yellow, red, green (1 item each)	10	140	100	1	4811111
1000	blue	10	167	125	12	482942
1000	yellow	10	167	125	12	482943
1000	red	10	167	125	12	482944
1000	green	10	167	125	12	482945
1000	Set: blue, yellow, red, green (1 item each)	10	167	125	1	4821111



## Graduated beakers, SAN



Crystal clear.

With molded graduations and stable, easy-grip handle.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
250	5	120	70	12	44091
500	10	133	91	12	44191
1000	10	170	116	6	44291
2000	20	215	150	6	44391
3000	50	242	170	6	44491



## Collectors, PP or SAN



With molded graduations. Volume: 2000 ml.

With stable, easy-grip handle and white PC lid.

Diameter: 150 mm; height: 220 mm.

Description	Divisions ml	PU	Cat. No.
SAN, molded graduations (Picture 1)	20	6	97891
PP, molded graduations	20	6	978941
PP, molded, blue embossed graduations (Picture 2)	20	6	978081
Accessories for collectors			
Lid, PC		6	97791



# Measuring and transferring

## Buckets, PE-HD



White. Without spout. With division into 1 liter segments.  
Stable handle with reinforcement in the middle for comfortable carrying.  
Tightly closing, transparent snap-on lid made of PE-LD - please order separately.

Description	Volume l	Divisions l	Height mm	Ø mm	PU	Cat. No.
Bucket	5	1	240	250	1	96093
Bucket	10	1	300	290	1	96393
Lid	for 5 L				1	96293
Lid	for 10 L				1	96593



## Buckets with spout, PP



Transparent. With division into 1 liter segments.  
With stable handle and spout for easy emptying.  
Highly resistant to chemicals.  
Without lid.

Volume l	Divisions l	Height mm	Ø mm	PU	Cat. No.
12	1	330	310	1	96694
15	1	370	310	1	96794





## Measuring scoops, PP



White. Also suitable as weighing scoops. With precision formed filling edge and comfortable, stable handle. Easily readable volume quantities on the upper side of the handle.

Volume ml	Length mm	PU	Cat. No.
2	60	12	39194
5	82	12	39294
10	100	12	39394
25	135	12	39494
50	160	12	39594
100	200	12	39694
250	260	6	39794
500	315	6	39894
1000	385	6	39994



## Measuring scoops, PP, coloured



Measuring scoops in different colours. Also suitable as weighing scoops. With precision formed filling edge and comfortable, stable handle. Easily readable volume quantities on the upper side of the handle.

Volume ml	Colour	PU	Cat. No.
50	red	12	395940
50	ultramarine	12	395950
100	red	12	396940
100	gray	12	396943
100	black	12	396944
100	yellow	12	396946
100	blue	12	396950
100	green	12	396952
100	bright blue	12	396955
100	ultramarine	12	396956
250	red	6	397940
250	ultramarine	6	397950
100	Set: white, red, grey, black, yellow, blue, green, bright blue, ultramarine (1 item each)	1	3961111

# Measuring and transferring

## Scoops, PE-HD



Conical in shape with tapered filling edge.

Volume ml	Length mm	Colour	PU	Cat. No.
15	115	natural	12	40093
25	135	natural	12	40193
65	185	natural	12	40293
110	215	natural	12	40393
150	250	natural	12	40493
350	310	natural	6	40593
750	350	natural	6	40693
750	350	ultramarine	6	406950
750	350	black	6	406944
1250	400	natural	6	40793
1250	400	ultramarine	6	407950
1250	400	black	6	407944






## Spatula, PA

Glass-fibre reinforced. Double spatula or spatula spoon, with stable, easy to hold handle in the middle.


Description	Length mm	PU	Cat. No.
Double spatula	150	10	80594
Double spatula	180	10	80595
Spatula spoon	180	10	80596
Spatula spoon	210	10	80593

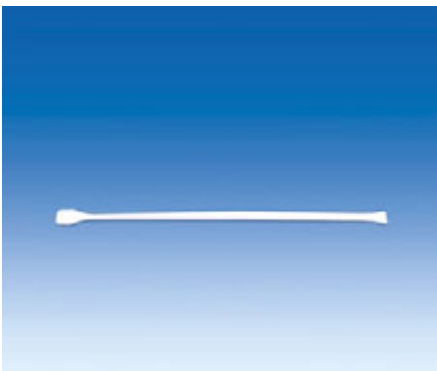

## Stirring rod, PP

Spatula-shaped extension for effective manual stirring of small volumes.

Length mm	PU	Cat. No.
245	10	80828

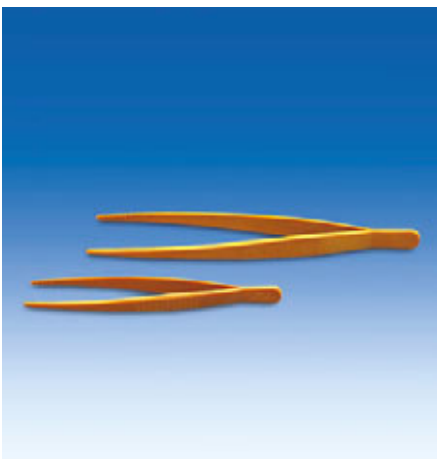

## Forceps, POM

Yellow, blunt, elastic, very good resilience. With grooves on the outside for optimum handling and grip.

Length mm	PU	Cat. No.
115	5	68099
145	5	68199
180	5	68299
250	5	68399



## Forceps, PMP



White, pointed, elastic, very good resilience.

Length mm	PU	Cat. No.
115	10	67895
145	10	67995



# Measuring and transferring

## Funnels, PP



Transparent. Rapid flow due to a steep 60° angle.  
Practical handle with loop for hanging.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	Stem length mm	PU	Cat. No.
5	30	45	1.5	25	24	40894
6	30	47	4	25	24	41094
14	40	65	4	35	24	41194
32	50	85	7	43	24	41294
88	75	108	7.2	55	12	41394
222	100	155	8	77	12	41494
342	120	180	11	90	12	41594
817	150	220	15	95	12	41694



## Powder funnels, PP



Transparent. With short, wide stem and practical tab for hanging. For transfer of powdered and granular substances. Rapid flow due to a steep 60° angle.

Ø mm	Length mm	Inner stem Ø mm	Stem length mm	PU	Cat. No.
65	70	15.5	26	10	70794
80	75	21	26	10	70894
100	92	24	23	10	70994
120	105	27.5	22	10	71094
150*	138	28	22	5	71194

\* Without tab





## Large funnels, PP



Transparent. Rapid flow due to a steep 60° angle. Practical handle for hanging. (Size 12500 ml without handle.) Suitable for filling large amounts of liquids. Optional accessories available: Stainless steel and aluminium sieve insert; however, not permissible for use with foodstuffs.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	PU	Cat. No.
1300	200	200	22	6	41794
3200	250	260	30	6	41894
12500	350	440	35	1	41994
Sieve insert Ø: 50 mm, for funnels no. 41794, 41894				1	42099



## Large funnels, PE-HD

Transparent. Rapid flow due to a steep 60° angle. Practical handle for hanging. Suitable for filling large amounts of liquids.

Volume approx. ml	Ø mm	Length mm	Inner stem Ø mm	PU	Cat. No.
12500	400	365	42	1	42294
17500	430	420	37	1	42393



## Standard joint funnels, PP



Transparent. For multi-neck flasks, laterally flattened, suitable for standard joint necks of various sizes. Suitable for the filling of liquid or powdered reagents into a reaction flask, especially for loading of multi-neck flasks during a reaction.

NS	Length mm	Wide opening mm	Stem length mm	PU	Cat. No.
14/23	75	40	17	10	70494
19/26	95	50	23	10	70594
29/32	135	75	30	5	70694

# Competence in Plastic Labware

SAMPLE PREPARATION




**VITLAB**   
Competence in Labware

# VITsafe™ - the Safety Wash Bottle


Working with chemical substances, which are sometimes dangerous, requires a high level of responsibility and concentration. With the VITsafe™ safety wash bottles VITLAB offers laboratory equipment that provides safety in the highest degree.

## VENT-CAP virtually prevents leakage

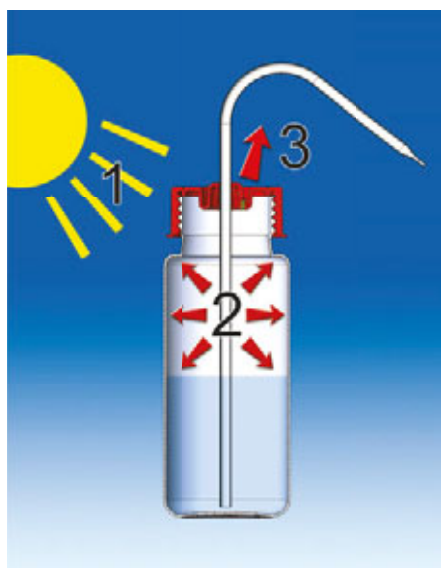

Temperature changes **(1)** in a laboratory can often cause conventional wash bottles to leak or drip due to the resulting increase in internal pressure **(2)**. The patent-registered, metal-free VENT-CAP screw closure of the VITsafe™ safety wash bottle virtually prevents this. The expansion of the gas due to the rise in pressure can escape through an integrated capillary **(3)**, thus dissipating the static over pressure. In addition, the lack of a spray insert allows turbulences to be almost completely avoided. The smooth and finely drawn tip of the spray bottle allows a precise spray jet and optimizes the fluid backflow. Dripping is subsequently almost entirely prevented.

## Clear identification due to safety imprint

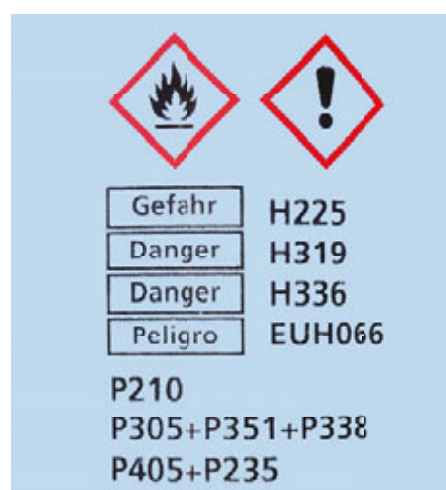

The permanent imprint according to directive (EC) No. 1272/2008 **(GHS)** offers even more safety.

It contains all essential information:

- Substance name in German, English, French and Spanish
- Chemical formula and CAS number
- Hazard pictogram with signal word
- Hazard (H) and precautionary (P) statements
- as well as the U.S.-based NFPA diamond

The VITsafe™ safety wash bottles are available as narrow-mouth or wide-mouth type. The particularly large opening of the wide-mouth bottles allows filling even without a funnel. Select the safety wash bottles to fit your applications from among **17 different substance names** and three volumes (250/500/1000 ml).



# Sample preparation

## VITsafe™ safety wash bottles, narrow-mouth



Bottle made of PE-LD (or PP for acetone and MEK), PP spray tube.

More safety due to the durable safety imprint in accordance to Directive (EC) No. 1272/2008 (GHS), as well as with all important information:

- Material name in German, English, French and Spanish
- Chemical formula, CAS No., hazard pictogram, signal word
- Risk phrases (H phrases), safety phrases (P phrases), as well as NFPA Code


Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube. Practically no leakage or dripping with the VENT-CAP screw cap, the design of which prevents almost all static overpressure.



Imprint	Colour VENT-CAP	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
Acetic acid	Red	500	25	180	74	6	1332979
Acetone	Red	250	25	135	65	12	1431829
Acetone	Red	500	25	180	74	12	1432829
Acetone	Red	1000	32	215	92	12	1433829
Acetonitrile	Red	500	25	180	74	6	1332969
Distilled Water	Blue	250	25	135	65	12	1331819
Distilled Water	Blue	500	25	180	74	12	1332819
Distilled Water	Red	1000	32	221	92	12	1333819
Ethanol	Orange	250	25	135	65	12	1331869
Ethanol	Orange	500	25	180	74	12	1332869
Ethanol	Red	1000	32	221	92	12	1333869
Ethyl acetate	Red	250	25	135	65	12	1331859
Ethyl acetate	Red	500	25	180	74	12	1332859
Ethyl acetate	Red	1000	32	221	92	12	1333859
Heptane	Red	500	25	180	74	6	1332899
i-Hexane	Red	500	25	180	74	6	1332909
Isopropanol	Yellow	250	25	135	65	12	1331849
Isopropanol	Yellow	500	25	180	74	12	1332849
Isopropanol	Red	1000	32	221	92	12	1333849
Methanol	Green	250	25	135	65	12	1331839
Methanol	Green	500	25	180	74	12	1332839
Methanol	Red	1000	32	221	92	12	1333839
Methyl ethyl ketone (MEK)	Red	500	25	180	74	6	1432989
Methylene chloride	Red	500	25	180	74	6	1332879
N,N-Dimethylformamide	Red	500	25	180	74	6	1332889
Pentane	Red	500	25	180	74	6	1433959
Tetrahydrofuran (THF)	Red	500	25	180	74	6	1332939
Toluene	Red	500	25	180	74	6	1332949
Xylene	Red	500	25	180	74	6	1332959

\* Height without spray tube

Other variations available upon request.

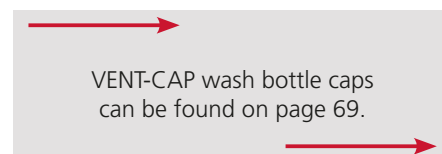



## VITsafe™ safety wash bottles, wide-mouth

Bottle made of PE-LD (or PP for acetone and MEK), PP spray tube.

More safety due to the durable safety imprint in accordance to Directive (EC) No. 1272/2008 (GHS), as well as with all important information:

- Material name in German, English, French and Spanish
- chemical formula, CAS No., hazard pictogram, signal word
- Risk phrases (H phrases), safety phrases (P phrases), as well as NFPA Code

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube. Practically no leakage or dripping with the VENT-CAP screw cap, the design of which prevents almost all static overpressure.

VENT-CAP wash bottle caps  
can be found on page 69.

Imprint	Colour VENT-CAP	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
Acetic acid	Red	500	45	166	76	6	1352979
Acetone	Red	250	45	146	58	12	1451829
Acetone	Red	500	45	166	76	12	1452829
Acetone	Red	1000	63	226	91	12	1453829
Acetonitrile	Red	500	45	166	76	6	1352969
Distilled Water	Blue	250	45	146	58	12	1351819
Distilled Water	Blue	500	45	166	76	12	1352819
Distilled Water	Red	1000	63	226	91	12	1353819
Ethanol	Orange	250	45	146	58	12	1351869
Ethanol	Orange	500	45	166	76	12	1352869
Ethanol	Red	1000	63	226	91	12	1353869
Ethyl acetate	Red	250	45	146	58	12	1351859
Ethyl acetate	Red	500	45	166	76	12	1352859
Ethyl acetate	Red	1000	63	226	91	12	1353859
Heptane	Red	500	45	166	76	6	1352899
i-Hexane	Red	500	45	166	76	6	1352909
Isopropanol	Yellow	250	45	146	58	12	1351849
Isopropanol	Yellow	500	45	166	76	12	1352849
Isopropanol	Red	1000	63	226	91	12	1353849
Methanol	Green	250	45	146	58	12	1351839
Methanol	Green	500	45	166	76	12	1352839
Methanol	Red	1000	63	226	91	12	1353839
Methyl ethyl ketone (MEK)	Red	500	45	166	76	6	1452989
Methylene chloride	Red	500	45	166	76	6	1352879
N,N-Dimethylformamide	Red	500	45	166	76	6	1352889
Pentane	Red	500	45	166	76	6	1453959
Tetrahydrofuran (THF)	Red	500	45	166	76	6	1352939
Toluene	Red	500	45	166	76	6	1352949
Xylene	Red	500	45	166	76	6	1352959

\* Height without spray tube

Other variations available upon request.



# Sample preparation

## VENT-CAP wash bottle caps, PP

Screw cap and spray tube from PP.

Practically no leakage or dripping with the VENT-CAP screw cap, the design of which prevents almost all static overpressure.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Thread GL	Colour	PU	Cat. No.
25	Red	12	833019
32	Red	12	833029
45	Red	12	833039
63	Red	12	833049
25	Blue	12	833085
25	Green	12	833086
25	Orange	12	833089
25	Yellow	12	833088
45	Blue	12	833095
45	Green	12	833096
45	Orange	12	833099
45	Yellow	12	833098



## Wash bottles with imprint, PE-LD/PP



Narrow- / wide-mouth bottles made of PE-LD, transparent.

Screw cap and spray tube from PP.

Imprinted with "Distilled Water" in German, English, French and Spanish.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Upon request, also with other imprints for non-hazardous media according to the REACh Directive.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	135	65	12	133181
250	45	146	58	12	135181
500	25	180	74	12	133281
500	45	166	76	12	135281
1000	32	221	92	12	133381
1000	63	226	91	12	135381

\* Height without spray tube



Wash bottles made from PE-LD/PP with no imprint, transparent and coloured, can be found on page 71.



## PFA-economy wash bottles



“PFA-economy” quality wash bottles. Transparent.

With recycled PFA content. Thus, reasonably priced and environmentally friendly.

PFA-economy bottles have excellent chemical resistance and high thermal stability and can be used for less critical applications for which pure PFA is not necessary.

Screw cap made from ETFE, spray tube from FEP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	157	61	1	108792
500	25	189	76	1	108892
1000	32	233	96	1	108992

\* Height without spray tube



## Wash-bottles, PP



Narrow- / wide-mouth bottles made of PP, transparent. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
250	25	135	65	12	94993
250	45	146	58	12	93793
500	25	180	74	12	95093
500	45	166	76	12	93993
1000	32	215	92	12	95193
1000	63	226	91	12	94193

\* Height without spray tube

# Sample preparation

## Wash-bottles, PE-LD/PP



Narrow- / wide-mouth bottles made of PE-LD, transparent. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
50	18	85	37	24	94588
100	18	114	43	24	94688
250	25	135	65	12	94988
250	45	146	58	12	93788
500	25	180	74	12	95088
500	45	166	76	12	93988
1000	32	221	92	12	95188
1000	63	226	91	12	94188

\* Height without spray tube



Wash bottles with imprint can be found on page 69.

## Wash-bottles, coloured, PE-LD/PP

Narrow-mouth bottles, made from PE-LD. Available in four different colours to facilitate ready identification. Screw cap and spray tube from PP.

Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Colour	Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
red	250	25	135	65	5	132603
red	500	25	180	74	5	132703
red	1000	32	221	92	5	132803
green	250	25	135	65	5	132605
green	500	25	180	74	5	132705
green	1000	32	221	92	5	132805
yellow	250	25	135	65	5	132606
yellow	500	25	180	74	5	132706
yellow	1000	32	221	92	5	132806
blue	250	25	135	65	5	132608
blue	500	25	180	74	5	132708
blue	1000	32	221	92	5	132808
Set: red, green, yellow, blue (1 item each)	500	25	180	74	1	1327111
Set: red, green, yellow, blue (1 item each)	1000	32	221	92	1	1328111

\* Height without spray tube






## Wash-bottles, PE-LD

Narrow-mouth bottles, transparent, with screw cap. Spray tube and spray-tube insert made from PE-LD. The classic model, made from soft material with good restoring force.

Volume ml	Thread GL	Height* mm	Ø mm	PU	Cat. No.
100	18	106	45	50	134293
250	25	140	59	50	134393
500	25	180	75	50	134493
1000	28	212	94	25	134593

\* Height without spray tube

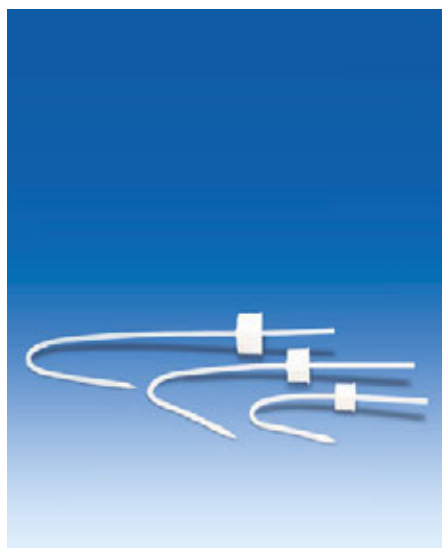

## Wash bottle caps, PP

Screw cap and spray tube with drawn-out tip, made of PP. Precise spray jet and optimised medium backflow through the continuous and finely drawn tip of the spray tube.

Thread GL	PU	Cat. No.
18	24	83300
25	12	83301
32	12	83302
45	12	83303
63	12	83304

# Sample preparation

## Dropping bottles, PE-LD/PE-HD



Narrow-mouth bottles made of PE-LD, transparent, with dropper insert and screw cap made from PE-HD.

Extra long, fine dropping tip for accurate dispensing.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	129	37	24	94587
100	18	155	43	24	94687
250	25	183	65	12	94987
500	25	228	74	12	95087
1000	32	269	92	12	95187



## Caps with dropper inserts, PE-HD



For bottles with GL threads. Cap with dropper insert, complete with screw cap made from PE-HD.

Extra long, fine dropping tip for accurate dispensing.

Thread GL	PU	Cat. No.
18	24	83306
25	12	83307
32	12	83308




## Dropping bottles, PE-LD

Narrow-mouth bottles, transparent, with dropper insert and red screw cap made of PE-LD. The classic model, made from soft material with good restoring force.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
20	14	88	31	100	132193
30	14	96	34	100	132293
50	18	115	39	100	132393
100	18	136	45	50	132493
250	25	170	59	50	132593
500	25	209	75	50	132693
1000	28	240	94	25	132793



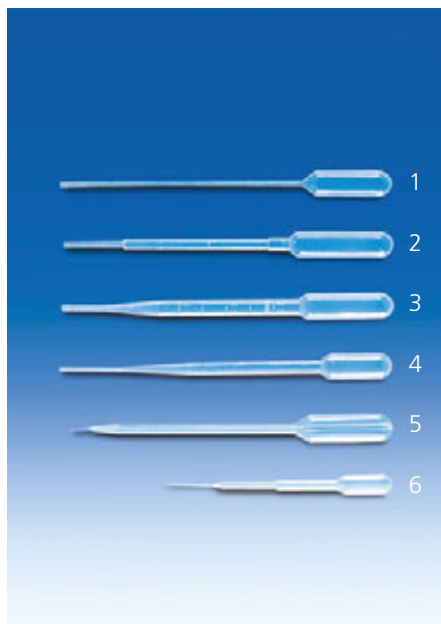

## Pasteur pipettes, PE-LD

Disposable. Very good reproducibility of the number of drops per milliliter, thus ideal for distributing aliquots of liquid portions. Pasteur pipettes can be deep-frozen when filled, or if needed, be converted into sealed vessels through heat-sealing. The integrated suction bulb can readily be compressed. Thus, finger fatigue from frequent pipetting is avoided. Can be sterilised with gas or gamma radiation.

Figure No.	Material	Graduations/ divisions ml	Max. suction volume ml	Tip outer Ø mm	Length mm	Number of drops per ml	PU	Cat. No.
1	PE-LD	-	3.0	2.8	152	25-27	5000	148893
2	PE-LD	1/0.25	3.5	3.4	151	25-30	5000	148993
3	PE-LD	3/0.5	3.5	3.2	152	21-28	5000	149093
4	PE-LD	2/0.5	2.0	3.3	152	22-26	5000	149193
5	PE-HD	-	4.0	3.0	150	25	5000	149293
6	PE-HD	0.25	1.0	1.0	144	70	5000	149393



## Dropping pipettes, PE-LD

With integrated bellows.  
For sampling and decanting of infectious or toxic liquids.  
Graduated.

Volume ml	Length mm	PU	Cat. No.
1.5	134	100	149893
5	195	100	149993



## Dropping pipettes, PE-LD

With integrated pipetting bulb.  
For sampling and decanting of infectious or toxic liquids.  
Without graduations.

Volume ml	Length mm	PU	Cat. No.
1.8	98	250	149693



# Sample preparation

## Spray bottles

White or transparent bottles made from PP and PE-LD.

Sprayer insert with stable, smoothly operated pump trigger and adjustable spray nozzle, which can be regulated from the finest mist (nebulising) to a precise liquid jet.

Range: approx. 3-4 meters.

For spraying detergents or disinfectants, especially into difficultly accessible areas, as well as applications in thin layer chromatography.

Volume ml	Colour	Material	PU	Cat. No.
400	white	PP	5	53510
850	white	PP	5	53610
1000	transparent	PP	5	95286
1000	transparent with imprint „Ethanol“*	PE-LD	5	952861

\* More information on imprint on page 66





## Griffin beakers, PFA



Transparent. With molded graduations. Excellent chemical resistance and very high thermal stability from -200 to +260 °C.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	32	1	110205
50	10	59	39	1	110305
100	20	72	50	1	110405
250	50	96	67	1	110605
500	100	122	88	1	110905
1000	100	141	109	1	111005

# Sample preparation

## Griffin beakers, ETFE



Transparent. With easily readable, printed black graduations. According to ISO 7056. Very good chemical resistance and very high thermal stability from -100 to +150 °C. To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	32	1	110204
50	10	59	39	1	110304
100	20	72	50	1	110404
250	50	96	67	1	110604
400	50	109	77	1	110704
500	100	122	88	1	110904
600	100	125	91	1	110804
1000	100	143	105	1	111004



## Griffin beakers, PTFE



White, opaque, thick-walled. Without scale. Excellent chemical resistance and high thermal stability from -200 to +260 °C. Also suitable for microwave ovens. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Wall thickness mm	Height mm	Ø mm	PU	Cat. No.
5	2	26	20	1	112197
10	2	33	24	1	112297
25	2	47	32	1	112397
50	2	60	43	1	112497
100	3	68	54	1	112597
250	3	97	66	1	112697
500	4	125	80	1	112797
1000	4	155	100	1	112897



Watch glasses  
can be found on page 80.



## Griffin beakers, PMP, printed red graduations

Crystal clear. With easily readable, printed red graduations.

According to ISO 7056.

To preserve markings, cleaning at no higher than 60 °C is recommended.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
10*	2	36	30	12	60503
25	5	50	38	12	60603
50	10	60	47	12	60703
100	10	70	55	12	60803
150*	20	80	66	12	60903
250	25	95	77	6	61003
400*	50	112	87	6	61103
500	50	118	94	6	61803
600*	50	127	100	6	61203
1000	100	147	120	6	61403
2000	200	187	149	6	61503
3000	250	212	170	4	61603
5000	500	247	203	4	61703

\* Variant in addition to ISO 7056



## Griffin beakers, PMP, molded graduations



Crystal clear. With molded graduations.

According to ISO 7056.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	38	12	60695
50	10	60	47	12	60795
100	10	70	55	12	60895
150*	20	80	66	12	60995
250	25	95	77	6	61095
400*	50	112	87	6	61195
500	50	118	94	6	61895
600*	50	127	100	6	61295
1000	100	147	120	6	61495
2000	200	187	149	6	61595
3000	250	212	170	4	61695
5000	500	247	203	4	61795

\* Variant in addition to ISO 7056

# Sample preparation

## Griffin beakers, PP, molded blue graduations



Highly transparent. With easily readable molded, embossed blue graduations.  
According to ISO 7056.

To preserve markings, do not clean at temperatures exceeding 60 °C.

Conditionally autoclavable at 121 °C (2 bar) according to DIN EN 285. For autoclaving we recommend the design with molded graduations (Cat. No. 606941 – 617941).

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
10*	2	36	30	12	605081**
25	5	50	38	12	606081**
50	10	60	47	12	607081**
100	10	70	55	12	608081
150*	20	80	66	12	609081
250	25	95	77	6	610081
400*	50	112	87	6	611081
500	50	118	94	6	618081
600*	50	127	100	6	612081
1000	100	147	120	6	614081
2000	200	187	149	6	615081
3000	250	212	170	4	616081
5000	500	247	203	4	617081

\* Variant in addition to ISO 7056

\*\* Blue printed graduations, not molded



## Griffin beakers, PP, molded graduations



Highly transparent. With molded graduations.

According to ISO 7056.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
25	5	50	38	12	606941
50	10	60	47	12	607941
100	10	70	55	12	608941
150*	20	80	66	12	609941
250	25	95	77	6	610941
400*	50	112	87	6	611941
500	50	118	94	6	618941
600*	50	127	100	6	612941
1000	100	147	120	6	614941
2000	200	187	149	6	615941
3000	250	212	170	4	616941
5000	500	247	203	4	617941

\* Variant in addition to ISO 7056



Watch glasses  
can be found on page 80.



## Measuring cup, PP

Transparent. Very durable. With molded graduations. Can be used as dispensing or lab beaker.  
Not a medical device.

Fitting lid made of PE - please order separately.

Description	Volume ml	Divisions ml	Height mm	Ø mm	PU	Cat. No.
Measuring cup	30	1	42	37	100	69394
Snap-on lid, white, PE					100	69493



## Watch glasses, PTFE



White. Without base.

High thermal stability and chemical resistance.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Ideal for use to cover beakers.

Ø mm	PU	Cat. No.
50	1	113197
75	1	113297
100	1	113397
125	1	113497



## Watch glasses, PP



Transparent. With base.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Ideal for use to cover beakers.

Ø mm	PU	Cat. No.
60	10	80452
80	10	80454
100	10	80455
118.5	10	80456



# Sample preparation

## Erlenmeyer flasks, PMP with PP screw cap



Transparent.

Ideal for use as a receiving vessel in titrations.

Well suited for storage and cultivation of cell cultures. Far safer than glass flasks for use in incubator shakers due to the break resistance of plastic. Suitable for microwaves.

To preserve markings, cleaning at no higher than 60 °C is recommended.



Volume ml	Divisions ml	Thread GL	PU	Cat. No.
50	10	40	6	66695
100	20	40	6	66795
250	50	52	6	66895
500	100	52	6	66995
1000	200	52	4	67095

## Erlenmeyer flasks, PP with PP screw cap



Transparent.

Well suited for storage and cultivation of cell cultures. Far safer than glass flasks for use in incubator shakers due to the break resistance of plastic. Suitable for microwaves.

To preserve markings, cleaning at no higher than 60 °C is recommended.



Volume ml	Divisions ml	Thread GL	PU	Cat. No.
50	10	40	6	666941
100	20	40	6	667941
250	50	52	6	668941
500	100	52	6	669941
1000	200	52	4	670941



## Magnetic stirring bars, polygonal, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates.

Ø mm	Length mm	PU	Cat. No.
2	5	5	300497
2	7	5	300597
3	8	5	300897
3	10	5	301097
3	13	5	301197
4.5	12	10	301597
6	10	10	301697
6	15	10	301797
6	25	10	301997
6	30	10	302097
7	20	10	301897
7	50	10	302297
7	60	10	302397
8	40	10	302197
10	70	5	302497
10	80	5	302597
27	57	1	303097
27	108	1	303197
27	159	1	303297



## Magnetic stirring bars, oval, PTFE



With permanent magnet AlNiCo V core. Highly suitable for vessels with a round bottom, such as round-bottom flasks. The angled side surfaces act to produce high turbulence, and thus achieve effective mixing.

Ø mm	Length mm	PU	Cat. No.
5	10	3	311097
6	15	3	311197
10	20	3	311297
12	25	3	311397
16	30	3	311497
16	35	3	311597
20	40	1	311697
20	50	1	311797

# Sample preparation

## Magnetic stirring bars, octagonal, PTFE



With rings and permanent magnet AlNiCo V core. The eight-sided shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates. The middle ring also promotes stable centering with convex or uneven bottoms.

Ø mm	Length mm	PU	Cat. No.
8	13	3	307697
8	15	3	307797
8	22	3	307897
8	25	3	307997
8	28	3	308097
8	38	3	308197
8	41	3	308297
8	51	3	308397
8	64	3	308497
10	13	3	308597
10	25	3	308897
10	35	3	308997
10	38	3	309097
10	51	3	309297
10	64	3	309397



## Magnetic stirring bars, cross shape, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates. The cross shape promotes very stable centering.

Size mm	Height mm	PU	Cat. No.
10 x 10	5	1	316097
20 x 20	8	1	316197
25 x 25	9	1	316297
30 x 30	10	1	316397
38 x 38	11	1	316497





## Magnetic stirring bars, triangular, PTFE



With permanent magnet AlNiCo V core. The angled shape gives rise to significant turbulence, and thus achieves effective mixing, even at low spin rates.

Edges mm	Length mm	PU	Cat. No.
6	12	3	310197
8	25	3	310297
14	40	3	310397
12	50	3	310497



## Magnetic stirring bars, barbell, PTFE



With permanent magnet AlNiCo V core. Excellent centering due to the small contact surface, and effective mixing. Disk diameter: 20 mm; shaft diameter: 8 mm.

Length mm	PU	Cat. No.
35	3	3125970
55	3	3126970



## Magnetic stirring bar retrievers, flexible, PTFE



Flexible magnetic stir bar retriever with a total length of 330 mm. Magnet encapsulated. Ø x L: 12.5 x 51 mm. Due to the high flexibility, the magnet stir bar can be retrieved from inaccessible locations, e.g., from the water trap in a laboratory sink. High chemical resistance, simple to clean.

Length mm	PU	Cat. No.
330	1	318597



## Magnetic stirring bar retrievers, PTFE



With PTFE encapsulated magnetic core. Straight shape. High chemical resistance, simple to clean.

Length mm	PU	Cat. No.
150	1	122097
250	1	122197
350	1	122297

# Sample preparation

## Magnetic stirring bar retrievers, PE



With a permanent magnet on one end and holding ring on the other one.  
Magnet is completely encapsulated in a PE mantle.

Length mm	PU	Cat. No.
300	1	318293
450	1	318393



## Mortars, MF

White, with spout. Stable circumferential edge. Very stable.

Volume ml	Height mm	Ø mm	PU	Cat. No.
300	75	125	5	72898
500	90	150	5	72998



## Pestles, MF

White, heavy design. with ergonomically shaped grip.

Length mm	Head Ø mm	PU	Cat. No.
125	30	5	73498
145	35	5	73598
160	40	5	73698
215	42	1	73898






## Urbanti funnels, PMP

Crystal clear. The spiral-shaped ribs increase the rate of filtration and prevent the trapping of air between the filter paper and the funnel. With long stem.

Volume approx. ml	Ø mm	Length mm	Stem Ø mm	Stem length mm	PU	Cat. No.
30	51	195	3	150	6	325095
80	70	210	3	150	6	325195
250	100	198	7	108	4	325295
630	140	247	10	132	3	325395
1800	196	315	20	155	2	325495

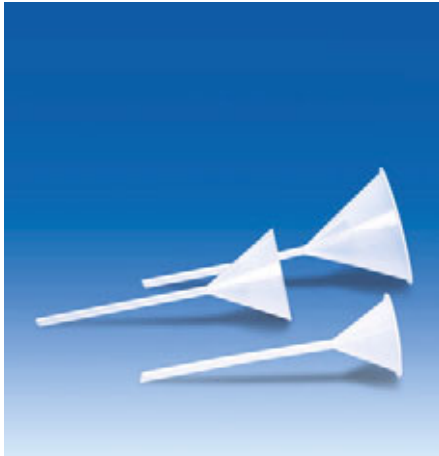

## Analytical funnels, PP

Transparent. With long stem and grooves. Rigidified by a thickened edge. Rapid flow due to a steep 60° angle.

Volume approx. ml	Ø mm	Length mm	Stem Ø mm	Stem length mm	PU	Cat. No.
50	50	194	5	150	10	80162
100	72	208	5	143	10	80164
225	91	227	5	145	10	80165



## Büchner funnels, PP

Two parts. Upper and lower parts are detachable to facilitate cleaning.

Volume approx. ml	Filter Ø mm	Length mm	Hole Ø mm	PU	Cat. No.
40	42.5	95	1.2	1	80437
70	55	113	1.1	1	80438
180	70	145	2.0	1	80439
280	80	165	2.0	1	80440
390	90	180	2.5	1	80441
810	110	210	2.5	1	80442
2100	160	280	2.75	1	80443
6000	240	350	3.0	1	80445



# Sample preparation – material separation

## Water-jet pump, PP

For generation of a vacuum and to siphon off liquids and vapours (if necessary, with a suction main or condensation trap connected upstream).

Pump fluid: Water

Length of the unit: approx. 210 mm (R 3/4" connector fitted)

Weight: approx. 33 g (R 3/4" connector fitted)

- High chemical resistance, since the pumped media only come into contact with polypropylene, FKM and PTFE.
- Operating temperature up to a maximum of 80 °C.
- Integrated non-return valve increases operating safety.
- Simple operation, and easy to clean.
- Detachable vacuum connection.
- Variety of supplied adapters simplify connections to most water sources, and additional reducing adapters are available.

Very low water consumption:

The flow configuration has been optimised, resulting in a 33% reduction of water consumption (approx. 220 liters/h at 3.5 bar water supply pressure).

Constant discharge pressure:

The discharge pressure of 16 mbar (water temperature: 12 °C) is reachable across a wide range of water supply pressures of from 3 to 6 bar.

High suction capacity:


The suction capacity is approx. 400 L/hour of air ( $\pm 50$  l/h, vs. atmospheric pressure, 12 °C water temperature, 3.5 bar water supply pressure).

Included in delivery:


Water jet pump, including: water supply connection (lock nut R 3/4", reducing adapter R 1/2" and hose connection (olive) with outer  $\varnothing$  10-12 mm), vacuum connection (olive with outer  $\varnothing$  6-9 mm, detachable with GL 14 screw cap).




Water consumption as function of water supply pressure

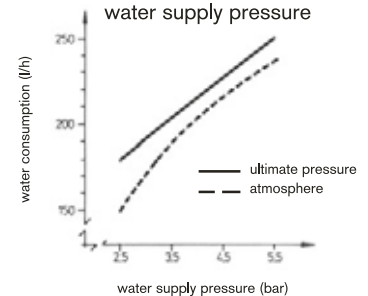

Ultimate pressure as function of water temperature

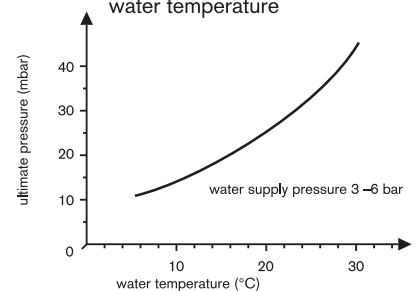

Pumping capacity as function of back pressure

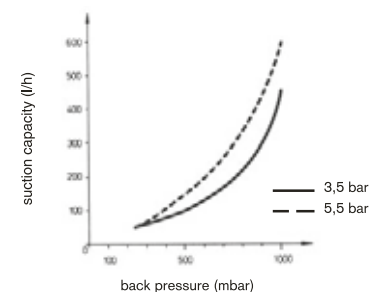

Description	PU	Cat. No.
Water-jet pump	1	77094
Accessories:		
Reducing adapter R3/4 inch to R3/8 inch	1	159665
Reducing adapter R3/4 inch to M 22x1, Perlator thread	1	159670



## Filtering racks

---

Funnel holder with base and adjustable height, made from PP, support stand made from stainless steel, diameter: 12.7 mm; and, length: 595 mm. To hold from two to four funnels with an upper outer diameter of 50-120 mm.

Positions	Base plate mm	PU	Cat. No.
2	250 x 140	1	78394
4	450 x 140	1	78294



## Support for separatory funnels, PP

---

For separatory funnels of from 125-500 ml. With practical clamps for simple attachment to stand rods with diameters of 8-14 mm.

Positions	PU	Cat. No.
1	5	80970

# Sample preparation – material separation

## Imhoff or sedimentation cone, SAN

According to DIN 12 672. Crystal clear, with molded graduations for precise reading of volumes. For simple, basic cleaning and rinsing, the screw coupling on the tip can be removed. Lower breakage risk than for PC or glass containers. For determination of suspended matter in liquids (e.g., for industrial and municipal wastewater).

Graduation:	Divisions:	Error limits:
0 - 2 ml	0.1 ml	+/- 0.1 ml
2 - 10 ml	0.5 ml	+/- 0.5 ml
10 - 40 ml	1 ml	+/- 1 ml
40 - 100 ml	2 ml	+/- 2 ml
100 - 1000 ml	50 ml	+/- 10 ml

Volume ml	PU	Cat. No.
1000	3	75991



## Sedimentation rack, PMMA

Holds two Imhoff sedimentation cones. Base plate with depression for exact vertical positioning of the sedimentation cone.

L x W x H mm	PU	Cat. No.
150 x 300 x 290	1	81056



## Evaporating dishes, PFA



With snap-on lid, PE. For contamination free sample preparation and efficient transportation. Due to a conical depression in the middle of the base very small amounts of a solvent are adequate to absorb the evaporated samples.

Volume ml	Height mm	Ø mm	PU	Cat. No.
25	25	50	1	103297
50	54	50	1	103397





## Round-bottom flasks, PFA



Transparent, neck with NS 29/32. Suitable as safety flask for use with rotary evaporators (operation at room temperature) to collect the distilled off liquid. High thermal stability and chemical resistance.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable.
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Height mm	Ø mm	PU	Cat. No.
100	117	65	1	107797
250	147	88	1	107897
500	177	107	1	107997



## Round-bottom flask stand, PP



White, for flasks with a round bottom. Excellent chemical resistance. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Ø mm	PU	Cat. No.
160	5	80271

# Sample preparation – material separation

## Gas wash bottles, PFA



Cap with S 40 buttress threads, and frit made of PTFE. A pore size of approx. 50 µm for optimal optimal pearling of the gas into the liquid. A wide field of application is possible due to the use of high-quality fluoroplastic. Suitable only for non-pressurised operation.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.



Volume ml	Height mm	Ø mm	Hose connection inner / outer Ø mm	PU	Cat. No.
250	160	61	4 / 6	1	159497
500	190	76	4 / 6	1	159597
1000	240	96	5 / 8	1	159697



## Desiccators with stopcock, PC

Crystal clear, with stopcock for evacuation. Lower sections can be filled with desiccants. The materials to be dried are placed on a perforated disc made of PP. Lid is sealed by a neoprene gasket. Ideal for use in educational laboratories.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
171	140	206	1	326496
230	190	260	1	326596
273	230	311	1	326696



## Desiccators, PP/PC

Lower portion made from PP can be filled with desiccants. The materials to be dried are placed on a perforated disc made of PP. The lid made from PC is sealed with a neoprene gasket. Ideal for use in educational laboratories.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
171	140	206	1	326094
230	190	260	1	326194
273	230	311	1	326294



## Desiccators with stopcock, PP/PC

With a bleed valve and an O-ring seal between the dome and the lower portion. The desiccators are suitable for vacuum and are provided with a non-return valve. Hot crucibles should only be placed on a porcelain plate, and should not come into too close contact with the rim of the desiccator. The insert made of PP serves to hold the drying agent. Desiccator plates should be purchased separately.

Ø mm	Disc Ø mm	Height mm	PU	Cat. No.
150	140.5	190	1	80550
200	189	230	1	80230
250	238	300	1	80554



# Sample preparation – material separation

## Desiccator plates, PP and porcelain

The PP plates are ideally suited for storage of crucibles and other containers at room temperature. The porcelain plates can also be used for hot crucibles.


Material	For desiccator Ø mm	Ø mm	PU	Cat. No.
PP	150	140.5	1	80551
PP	200	189	1	80231
PP	250	238	1	80553
Porcelain	150	140	1	65965
Porcelain	200	190	1	65975
Porcelain	250	235	1	65980



## Replacement parts for desiccators

Replacement O-rings and valves for desiccators (cat. nos. 80550, 80230, 80554).

Description	PU	Cat. No.
O-ring for desiccator no. 80550	1	80555
O-ring for desiccator no. 80230	1	80556
O-ring for desiccator no. 80554	1	80557
Valve, PC, for desiccator nos. 80550, 80230 and 80554	1	80229

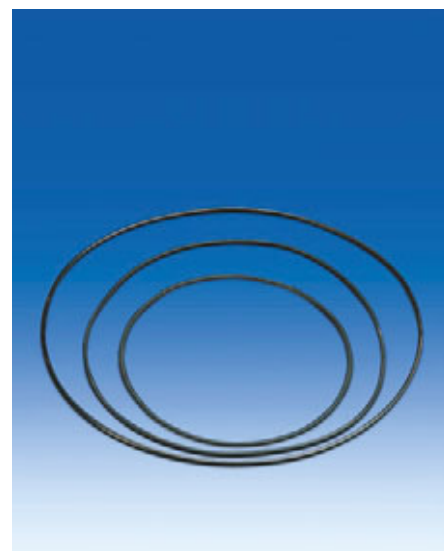



## Sample containers, PFA



With screw cap made of PFA. Cylindrical, tall shape.  
Ideal for sample collection, transport and storage of samples.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability from -200 °C to +260 °C, autoclavable at 121 °C (2 bar) according to DIN EN 285
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw material

Further information on PFA can be found starting on page 130.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
30	40	54	38	1	130297
60	40	90	38	1	130397
90	56	62	54	1	130497
180	56	112	54	1	130597



## Sample containers, PE-HD

With screw cap made of PE-HD. Cylindrical, tall shape.  
Ideal for sample collection, transport and storage of samples.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
5	23	36	21	10	80910
10	23	58	21	10	80911

# Sample preparation – material separation

## Sample containers, PP



Transparent. With screw cap made of PP. Cylindrical, tall shape.  
Ideal for sample collection, transport and storage of samples.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
30	40	54	38	10	130294
60	40	90	38	10	130394
90	56	62	54	10	130494
180	56	112	54	10	130594



## Sample containers, PP



Transparent. With snap-on lid made of PE-LD. Conical shape.

Volume ml	Height mm	Ø mm	PU	Cat. No.
5	25	20	25	68594
18	57	22	25	68894
50	97	30	10	69194
160	110	50	10	69294



## Sample containers, PE-LD

Transparent. With attached plug-seal cap made of PE-LD.

Volume ml	Height mm	Ø mm	PU	Cat. No.
1	32	8	500	80730
2.5	32	14	100	80731
5	50	15	100	80737
8	57	17	100	80732
10	32	22	100	80733
25	74	24	100	80734
30	52	31	50	80736
50	74	30	50	80735





## Weighing jars, PP

Transparent. With knobbed lid. Cylindrical shape.

Volume ml	Height mm	Ø mm	PU	Cat. No.
25	30	40	10	80342
30	50	30	10	80340
50	30	50	10	80345
65	35	60	10	80346
65	60	40	10	80343
200	90	60	10	80347
400	120	70	10	80348



## Sample tubes, PFA



Sample tubes made from PFA for sample preparation and for use in autosampler racks. With or without individually calibrated ring mark at 10 ml with GL 25 screw cap made from PFA or PE stopper (see Table).

The advantages of PFA:

- Especially suitable for use in trace analysis
- No memory effects
- Practically no carryover due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean

Further information on PFA can be found starting on page 130.

Figure Type No.		Volume ml	Height mm	Ø mm	PU	Cat. No.
1	With ring mark and screw cap	15	110	22	1	103897
-	Without ring mark	15	110	22	1	1038971
2	With ring mark and stopper	12	110	16	1	1037979
3	Without ring mark	12	110	16	1	103797

# Sample preparation – material separation

## Sample vials, PFA



Sample vials made of PFA with conical interior and molded graduation (5 ml subdivisions). Available in two different types, depending on application:

- Cored outside bottom
- Flat surface on bottom of vial for improved heat transfer (Recommended for use with hot plates)

Both 50 ml sizes fit in common Autosampler racks.

Scope of delivery is without screw cap. Please order the screw cap (Cat. No. 104997) separately.

Volume ml	Type outside bottom	Ø mm	Height* mm	PU	Cat. No.
15	Flat	29	39	1	104197
15	Cored	29	42	1	104097
25	Flat	29	69	1	104397
25	Cored	29	72	1	104297
50	Flat	29	117	1	104597
50	Cored	29	120	1	104497
Screw cap, 33 mm, PFA (suitable for sample vials (104097 – 104597)				1	104997

\* Height with thread



## Autosampler-vials, PFA



Molded graduation with 1 ml subdivisions.

Translucent material for optimum visibility of the liquid contained in the vial.

Conical interior for use with autosamplers. The outer design allows easy handling of the autosampler-vials with forceps. Optionally available with plug-seal cap for long term storage or lid with knob for fast opening and closing (dust protection) of the vial.

Scope of delivery is without lid or cap. Please order the fitting lid (Cat. No. 105597 resp. 105697) separately.

Volume ml	Ø mm	Height mm	PU	Cat. No.
1.5	13.5	24	1	105097
2.5	13.5	36	1	105197
4	14	52	1	105297
Plug-seal cap, PFA	18	5	1	105697
Lid with knob, PFA	16	9	1	105597




## Reagent tube racks, PP

White. For reagent tubes with a diameter of 21 mm.

With three levels for precise, vertical positioning of the reagent tubes.

Working temperatures of -20 to +90 °C.

For Ø up to mm	Positions	L x W x H mm	PU	Cat. No.
20	2 x 6	190 x 60 x 80	5	80560
20	2 x 12	375 x 65 x 95	5	80562

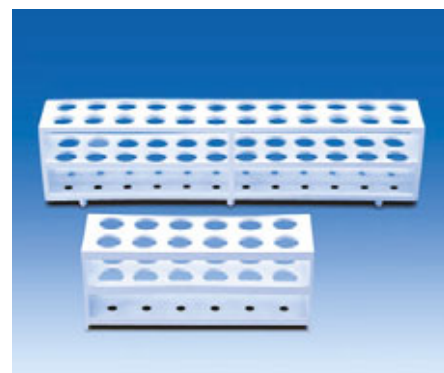

## Reagent tube racks, PP

White. The special shape makes it possible to check the amounts present in the reagent tubes.

With two side-mounted handle straps.

For Ø up to mm	Positions	L x W x H mm	PU	Cat. No.
16	10	200 x 55 x 65	4	80130
18	9	200 x 55 x 65	4	80131
Base plate for 2 reagent tube racks (Cat. No. 80130, 80131)		202 x 156 x 13.5	4	80134

## Test tube racks, PP, coloured

Stackable, simple, and small footprint. Alphanumerically identified positions. Suitable for tempering in a water bath as well as storage of samples in the refrigerator and incubation in a climate chamber. The racks are supplied as folded out flat, and can be firmly and inseparably joined together in just a few steps. Working temperatures of -20 to +90 °C.

Base area: 265 x 126 mm.

For Ø up to mm	Positions	Height mm	Colour	PU	Cat. No.
13	6 x 14	75	White	5	3190940
16	5 x 11	75	White	5	3191940
18	5 x 11	75	White	5	3192940
20	4 x 10	75	White	5	3193940
25	4 x 8	88	White	5	3194940
30	3 x 7	88	White	5	3195940
13	6 x 14	75	Blue	5	3190948
16	5 x 11	75	Blue	5	3191948
18	5 x 11	75	Blue	5	3192948
20	4 x 10	75	Blue	5	3193948
25	4 x 8	88	Blue	5	3194948
30	3 x 7	88	Blue	5	3195948
13	6 x 14	75	Red	5	3190943
16	5 x 11	75	Red	5	3191943
18	5 x 11	75	Red	5	3192943
20	4 x 10	75	Red	5	3193943
25	4 x 8	88	Red	5	3194943
30	3 x 7	88	Red	5	3195943

# Sample preparation – material separation

## Microtubes, PP



With attached plug-seal cap, with frosted labelling field. Subdivisions for reading the volume. The cap membrane has a uniform thickness and can be easily pierced by an analyzer. The attached plug-seal cap seals tightly and is firmly seated, yet reopens easily. The microtubes have a uniform wall thickness and are highly transparent. CE marked according to IVD Directive 98/79 EC.

- Can be centrifuged at an RCA of up to 20,000 RCF at 20 °C for up to 20 min
- Cap membrane Ø: 8.5 mm; approx. 0.3 mm thick
- Outer Ø x H: 10.75 x 40.8 mm

Volume ml	Packaging units	PU	Cat. No.
1.5	1 x 500	500	145094
1.5	6 x 500	3000	145194



## Microtube stands, PP



Opaque, gray. Numbered positions for 20 microtubes with volume of 1.5 ml. For working with samples as well as short- and medium-term storage. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Positions	L x W x H mm	PU	Cat. No.
20	210 x 70 x 37	1	3190941




## Microtube racks, PP, coloured

Stackable racks for micro- or cryotubes. Alphanumerically identified positions. Suitable for tempering in a water bath. The racks are supplied as folded out flat, and can be firmly and inseparably joined together in just a few steps. Working temperatures of -20 to +90 °C. Base area: 265 x 126 mm.

For Ø up to mm	Positions	Colour	Height mm	PU	Cat. No.
11	8 x 16	White	38	5	3197940
13	6 x 14	White	38	5	3198940
11	8 x 16	Blue	38	5	3197948
13	6 x 14	Blue	38	5	3198948
11	8 x 16	Red	38	5	3197943
13	6 x 14	Red	38	5	3198943





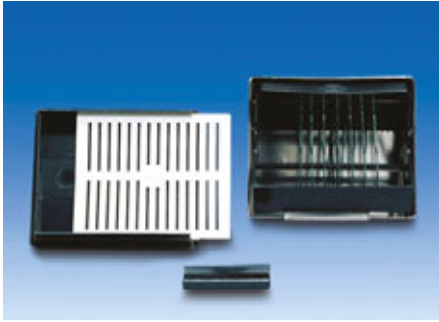

## Staining chamber for slides, POM

Consists of staining jar and a staining rack for 25 slides 76 x 26 mm.

L x W x H mm	PU	Cat. No.
100 x 87 x 51	5	99099



## Staining rack for slides, POM

For serial staining of 25 slides 76 x 26 mm.  
Usable in the staining jar, cat. no. 99199 (see below).

L x W x H mm	PU	Cat. No.
91 x 79 x 38	10	99299



## Staining jar for slides, POM

For combination with staining rack, cat. no. 99299 (see above).  
Can also be used as a storage box for 25 slides.

L x W x H mm	PU	Cat. No.
100 x 87 x 51	5	99199



## Slide storage boxes, PS

With lid. For 25, 50 or 100 slides, 76 x 26 mm. Handy, stackable, break resistant, easy to clean. The positions are numbered individually. With an index card.

Positions	L x W x H mm	PU	Cat. No.
25	122 x 96 x 34	4	80276
50	229 x 96 x 34	1	80277
100	229 x 181 x 34	1	80278



## Coplin staining chamber, PP

With screw cap made of PP, GL 45. For serial staining of 10 slides 76 x 26 mm.

Height mm	PU	Cat. No.
94	10	136693

# Competence in Plastic Labware

SAVING AND STORAGE WITH CONFIDENCE



**VITLAB**   
Competence in Labware

# VITgrip™ – The Allround Lab Bottle

The VITgrip™ lab bottles and screw caps of high-quality polypropylene (PP) are “Made in Germany”. VITgrip™ lab bottles are in many aspects a safe alternative to glass, as for example, the higher break resistance reduces the risk of injury and together with outstanding chemical resistance provides a long period of use.

## Leakproof\* and break resistant



Sometimes it happens very quickly: one inattentive moment and, by accident, the lab bottle is knocked over. Breakage of glass can be dangerous because of possible injury due to glass splinters and/or spilled liquid. VITgrip™ lab bottles made of plastic provide a higher level of safety in the lab because the VITgrip™ has a significantly higher break resistance and is leakproof\*. The bottle thread and the associated screw cap are an ideally matched pair. Together, they form a reliable sealing system without the need of an additional seal that can wear, corrode or cause contamination. Both components are subject to a detailed quality inspection prior to delivery.

## Safe storage



The VITgrip™ lab bottles are supplied with a tamper-evident closure; i. e. a ring, which is attached at the lower end of the screw cap will tear off upon the first opening of the closed bottle. It reliably signals, if the bottle is still sealed before opening. Thus, an intact tamper-evident closure can ensure safe storage of e. g. reference samples or safe transfer of samples between sampling site and lab. After the ring is torn off, the closure can be used as a regular screw cap. All VITgrip™ lab bottles have a GL 45 thread and an evenly formed neck area that allow controlled, smooth pouring of liquid.

# Saving and storing

## VITgrip™ lab bottles, PP, GL 45 with tamper-evident cap, PP



Everyday use bottles made of plastic for sampling and storing liquids in the lab.

Due to the innovative design and the ergonomic shape the bottles have an outstanding easy-grip feature. The slim and tapered shape greatly improves handling in comparison to conventional lab bottles. Furthermore, the molded volume graduations provide texture for an enhanced grip, especially when working with gloves.

Through the optimised sealing system of bottle threads and screw cap the bottle is leak-proof\* and offers an optimum pouring behaviour and easy cleaning due to the hydrophobic material and round shape.

With double-sided molded graduations (accuracy  $\pm 5\%$ ), the volume inside the bottle is easy to read, even during use.

The included tamper-evident cap reliably signals if the bottle is still sealed before opening.

The bottle has very good chemical resistance against most acids, bases and alcoholic solutions.



Volume ml	Graduation ml	Height** mm	Bottom-ø mm	PU	Cat.-No.
125	12.5	103	54	6	110194
250	25	149	64	6	110294
500	25	192	77	6	110394
1000	50	234	97	6	110494
2000	100	278	126	1	110594
Replacement tamper-evident cap, PP, GL 45				6	83330
Starter-Set (3 x VITgrip™ (250 / 500 / 1000 ml) + 3 x tamper-evident cap					111194

\* IMPORTANT NOTE: The term leakproof applies under the following test conditions:

The VITgrip™ lab bottle is half filled with distilled water and is closed with the supplied VITLAB® screw closure – after the ring of the tamper-evident closure clicks into place – with a torque of 5 Nm. Subsequently, the bottle is turned upside down and remains, standing on the screw cap, for 15 minutes, without the filled-in water escaping. The test is carried out at room temperature (approx. 20 °C) and atmospheric pressure.

\*\* Height without screw cap.



## Narrow-mouth bottles, PFA



Transparent.

With screw cap with buttress threads made of PFA. Ideal for long-term storage of high-purity oxidants, acids, alkalis, as well as hydrocarbons, trace analysis solvents and standards.

The advantages of PFA:

- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive, smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Use of high purity raw materials

Further information on PFA can be found starting on page 130.

Volume ml	Thread	Height mm	Ø mm	PU	Cat. No.
50	S 28	86	37	1	109297
100	S 28	120	45	1	109397
250	S 28	160	61	1	108297
500	S 28	190	76	1	108397
1000	S 28	240	96	1	108497



## Wide-mouth bottles, PFA



Transparent.

With screw cap made of PFA with buttress threads. Ideal for long-term storage of high-purity oxidants, acids, alkalis, as well as hydrocarbons, trace analysis solvents and standards.

Volume ml	Thread	Height mm	Ø mm	PU	Cat. No.
250	S 40	150	61	1	109497
500	S 40	179	76	1	109597
1000	S 40	217	96	1	109697
2000	S 40	245	130	1	109797

# Saving and storing

## PFA-economy narrow-mouth bottles



Narrow-mouth, "PFA-economy" quality wash bottles. Transparent.  
With recycled PFA content. Thus, reasonably priced and environmentally friendly.  
PFA-economy bottles have excellent chemical resistance and high thermal stability and can be used for less critical applications for which pure PFA is not necessary.  
With screw cap made of ETFE.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	90	37	1	108092
100	18	114	45	1	108192
250	25	157	61	1	108292
500	25	189	76	1	108392
1000	32	233	96	1	108492



## Screw caps, PFA



Transparent. For sealing all PFA containers with GL threads or buttress threads.  
Autoclavable at 121 °C (2 bar) according to DIN EN 285.

The advantages of PFA:

- Especially suitable for use in trace analysis
- Ideal for sensitive and valuable samples
- Long-term maintenance of low-concentration reference materials in PFA containers
- No memory effects
- Practically no carryover, no cross-contamination due to the extremely hydrophobic, anti-adhesive and smooth surfaces
- High thermal stability, from -200 °C to +260 °C, autoclavable
- Chemical inertness against nearly all chemicals
- Good transparency and dimensional stability
- Easy to clean
- Highly pure starting materials used

Further information on PFA can be found starting on page 130.

Thread	PU	Cat. No.
GL 18	1	102597
GL 25	1	102397
S 28	1	102697
S 40	1	102897







## Wide-mouth bottles, PTFE



White. Opaque. Thick walled.  
 With screw cap made of PTFE.  
 Very high thermal stability and chemical resistance.  
 With very wide mouth, ideal for filling with powders and paste-like materials.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
10	12	50	26	1	122597
25	19	61	33	1	122697
50	25	76	43	1	122797
100	35	88	52	1	122897



## Narrow-mouth bottles, PP



Transparent. With high shoulders.  
 With screw cap made of PP.  
 Good chemical resistance, ideal for long-term storage of liquids.  
 Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
250	25	135	65	12	94994
500	25	180	74	12	95094
1000	32	215	92	12	95194



## Wide-mouth bottles, PP



Transparent.  
 With screw cap made of PP.  
 Good chemical resistance, ideal for long-term storage of liquids.  
 Autoclavable at 121 °C (2 bar) according to DIN EN 285.  
 Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
250	45	146	58	12	93794
500	45	166	76	12	93994
1000	63	226	91	12	94194



# Saving and storing

## Narrow-mouth bottles, PE-LD



Transparent. With high shoulders.

With screw cap made of PP.

Flexible material with good resilience.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	18	85	37	24	94589
100	18	114	43	24	94689
250	25	135	65	12	94989
500	25	180	74	12	95089
1000	32	221	92	12	95189



## Wide-mouth bottles, PE-LD



Transparent.

With screw cap made of PP.

Flexible material with good resilience.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	32	87	39	24	93389
100	32	94	47	24	93489
250	45	146	58	12	93789
500	45	166	76	12	93989
1000	63	226	91	12	94189



## Screw caps, PP



Transparent. Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Thread GL	PU	Cat. No.
18	24	83310
25	12	83311
32	12	83312
40	12	83315
45	12	83313
52	12	83316
56	12	83317
63	12	83314





## Narrow-mouth bottles, PE-LD

Transparent. With flat shoulders.  
With screw cap made of PE-LD.  
Flexible material with good resilience.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
10	14	50	26	100	138093
20	14	58	31	100	138193
30	14	66	34	100	138293
50	18	85	39	100	138393
100	18	106	45	50	138493
250	25	140	59	50	138593
500	25	180	75	50	138693
1000	28	212	94	25	138793
2000	28	264	117	25	138893



## Wide-mouth bottles, PE-LD

Transparent.  
With screw cap made of PE-LD.  
Flexible material with good resilience.  
Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
50	32	80	38	100	139393
100	32	94	48	50	139493
250	40	126	62	50	139593
500	50	155	76	50	139693
1000	65	208	93	25	139793
2000	65	246	120	25	139893

# Saving and storing

## Narrow-mouth bottles, PE-HD

Transparent.

With screw cap made of PE-LD.

Small footprint due to the square cross-section and the high shoulders.

Volume ml	Thread GL	Height mm	Size mm	PU	Cat. No.
100	25	76	43 x 43	24	91789
250	28	80	80 x 80	24	91989
500	32	106	90 x 90	12	92089
1000	32	187	80 x 80	12	92189



## Wide-mouth bottles, PE-HD

Transparent.

With screw cap made of PE-LD.

Small footprint due to the square cross-section and the high shoulders.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread GL	Height mm	Size mm	PU	Cat. No.
100	32	78	46 x 46	24	92489
250	50	83	80 x 80	24	92689
500	65	120	90 x 90	12	92789
1000	65	168	90 x 90	12	92889



## Wide-mouth bottles, PE-LD, with eye closure

Transparent.

With eyes on the bottle and the screw cap for sealing.

With sealing plug and screw cap made of PP.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Volume ml	Thread mm	Height mm	Ø mm	PU	Cat. No.
50	24	75	40	25	80408
100	24	90	50	25	80409
250	36	130	60	25	80410
500	36	160	75	10	80411
1000	50	200	95	10	80412
2000	50	250	115	10	80413





## Reagent bottles, PP



Transparent.

With screw cap made of PP.

Good chemical resistance, ideal for storage of liquids.

Autoclavable at 121 °C (2 bar) in compliance with DIN EN 285, except for sizes 5000 and 10000 ml.

Volume ml	Thread GL	Height mm	Ø mm	PU	Cat. No.
100	18	100	52	20	100389
100	32	96	55	20	101589
250	25	132	70	20	100489
250	45	132	73	20	101689
500	25	165	87	10	100589
500	45	172	87	10	101789
1000	32	202	108	10	100689
1000	45	197	105	10	102089
1000	63	204	108	10	101889
2000	32	245	131	6	100789
2000	45	241	131	6	102189
2000	63	243	131	6	101989
5000*	45	315	178	1	100889
10000**	63	394	222	1	100989

\* with handle, PE-HD

\*\* with PE foam seal and two handles, PE-HD

# Saving and storing

## Reagent bottles, PP



Transparent.

With NS stopper made of PP.

Stopper type A: With square-knob cap and red core.

Stopper type B: With octagonal-knob cap and red core.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Volume ml	Neck NS	Height mm	Ø mm	Stopper	PU	Cat. No.
100	14/23	106	52	A	20	100394
100	29/32	111	55	B	20	101594
250	19/26	138	70	A	20	100494
250	34/35	144	73	B	20	101694
500	24/29	172	87	A	10	100594
500	45/40	183	87	B	10	101794
1000	29/32	213	108	A	10	100694
1000	60/46	214	108	B	10	101894



## Reagent bottles, opaque, PP, wide mouth



Transparent. Made from opaque, pigmented PP for light-sensitive substances.

According to DIN 12039.

With NS stopper made of PP.

Good chemical resistance, ideal for long-term storage of liquids.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

Wider mouth for simple filling, also ideal for powders and paste-like materials.

Further information on our opaque products can be found on page 132.

Volume ml	Neck NS	Height mm	Ø mm	PU	Cat. No.
500	45/40	183	87	10	1017940
1000	60/46	214	108	10	1018940



**VITLAB® opaque replaces brown glass** and is...

- ... substantially lighter in weight
- ... practically unbreakable
- ... practically impermeable in the UV region
- ... comparable to a light protection factor of 20



## Standard joint stoppers, PP



Stopper type A: With square-knob cap and red core.

Stopper type B: With octagonal-knob cap and red core.

Autoclavable at 121 °C (2 bar) according to DIN EN 285.

NS	Model	PU	Cat. No.
10/19	A	1	90694
12/21	A	1	90794
14/23	A	1	90894
19/26	A	1	90994
24/29	A	1	91094
29/32	A	1	91194
29/32	B	1	92194
34/35	B	1	91294
45/40	B	1	91394
60/46	B	1	91494

# Saving and storing

## Storage bottles, PE-HD, without tap

Transparent.

With stable carrying handle and screw cap.

Available in wide- and narrow-mouth models.

Volume l	Neck inner Ø mm	Height mm	Ø mm	PU	Cat. No.
5	90	318	163	1	81640
5	45	335	163	1	81644
10	120	390	205	1	81642
10	55	415	205	1	81646



## Storage bottles, PE-HD, with tap

Transparent. Narrow-mouth model.

With stable carrying handle and screw cap. The 25 and 50 l sizes come equipped with two carrying handles.

Complete with exchangeable, easily operated tap made from PP with a 3/4" pipe fitting.

Volume l	Neck inner Ø mm	Height mm	Ø mm	PU	Cat. No.
5	45	335	163	1	81660
10	55	415	205	1	81662
25	79.5	565	280	1	81664
50	79.5	700	350	1	81666



## Tap for storage bottles, PP

Replacement tap for storage bottles made from PP (Cat. No. 81660 to 81666).

Complete with 3/4" pipe fitting and rubber ring.

Description	PU	Cat. No.
Tap for storage bottles	1	80375







## Container, PP

Ideal for low-footprint storage of media. The rectangular shape means that the containers can be lined up side by side with no wasted space. Each container is supplied with a scale. With a wide opening for filling. Comfortable, simple dispensing of media with the easily operated dispensing and discharge tap. Dripping is prevented with the rotatable spout. Container supplied without stopcock.

Capacity: 5 L

Measurements: 65 x 335 x 335 mm

Filling opening diameter: 41 mm

Description	PU	Cat. No.
Rectangular carboy	10	155094
Vented screw cap	1	155594
Filling tap	1	156094



## Chemical waste disposal system, PE/PP

For collection of liquid chemicals in the laboratory. The inlet hopper made from PE-HD contains a self-closing float, overflow protection, and a splash guard. Additionally, a screw cap (GL 63) with sealing ring is included.

Volume l	Height mm	Ø mm	PU	Cat. No.
10	560	222	1	151594

# Saving and storing

## Bowl, PP, with lid



White. Rectangular shape.

Broad, stable, easy to grip edge.

Especially easy to clean due to the rounded corners and edges and the smooth surfaces.

Volume l	L x W x H mm	PU	Cat. No.
17	430 x 331 x 195	1	43610



## Transport containers, PE-HD

Transparent.

Easy stackable.

With reinforcing ribs and integrated carrying handles.

Broad, stable edge.

Volume l	L x W x H mm	PU	Cat. No.
20	420 x 310 x 205	1	80602
46	600 x 365 x 260	1	80603
72	700 x 420 x 310	1	80604



## Multi-purpose container, SAN

Crystal clear, with fitted lid. Planar bottom inside, reinforced edge outside for stable placement on the lab bench.

Ideal for dust-proof storage of small components, instruments and utensils.

Volume ml	L x W x H mm	PU	Cat. No.
4000	340 x 230 x 94	1	36491





## Dishes, PVC

White. All-purpose. Rounded corners and edges. Easy to clean.

Inner bottom dimensions mm	Height mm	PU	Cat. No.
200 x 150	50	1	80280
250 x 200	60	1	80281
320 x 260	75	1	80282
350 x 300	85	1	80283
430 x 330	95	1	80284
520 x 420	100	1	80285
675 x 530	110	1	80286
540 x 420	190	1	80288



## Laboratory trays / catchment trays, PP



White. All-purpose. Robust design. Very good chemical resistance  
Rounded corners and edges. Smooth surfaces, easy to clean.

Inner bottom dimensions mm	Edge dimensions mm	Height mm	PU	Cat. No.
130 x 180	180 x 230	42	1	165094
180 x 240	250 x 310	65	1	165194
240 x 300	310 x 370	75	1	165294
300 x 400	420 x 520	120	1	165394
400 x 500	534 x 634	140	1	165494
500 x 700	648 x 846	160	1	165594



## Bowls, PP



White. Round. With broad, stable edge and circumferential standing ring on the bottom.


Volume l	Height mm	Ø mm	PU	Cat. No.
0.9	70	160	5	42594
1.7	80	200	5	42694
2.9	100	240	5	42794
4.3	120	280	5	42894
6.6	130	320	3	42994
9.2	150	360	3	43094
13.4	180	400	3	43194

# Competence in Plastic Labware

LAB ASSISTANTS




**VITLAB**   
Competence in Labware

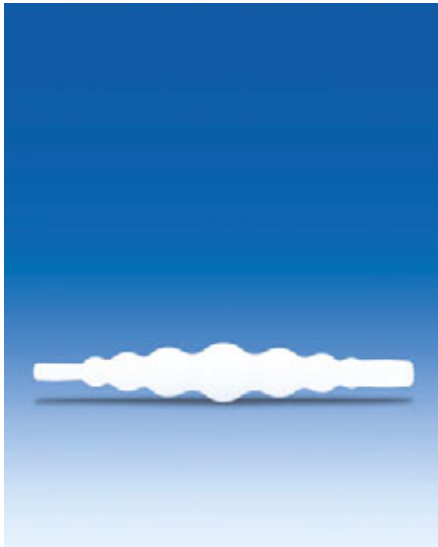

## Connectors, universal, PP

Due to its special shape, it can be used for a wide variety of different tubing inner diameters.

For tubing with an inner Ø of mm	PU	Cat. No.
5 - 15	10	78794

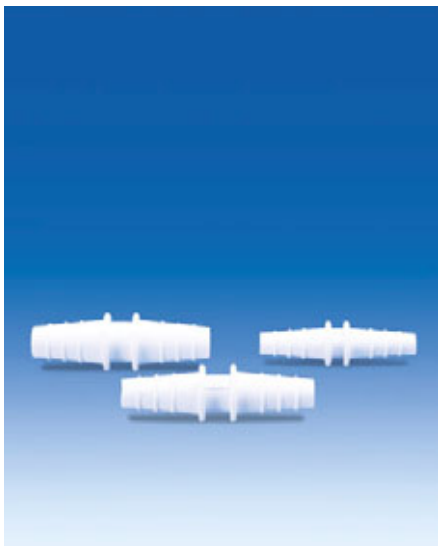

## Connectors, straight, PP

Conical shape to accept tubing of various inner diameters.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3 - 5	2.0	20	80510
5 - 7	3.5	20	80511
7 - 10	4.5	20	80512
9 - 12	6.5	20	80513
11 - 14	8.5	20	80514
13 - 16	10.5	20	80515



## Connectors, straight, PP

Conical shape, stepped. With different fitting diameters on the two sides to be able to connect with tubing having different diameters.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
4 - 8 / 8 - 12	1.6 / 4.6	20	80877
4 - 8 / 12 - 16	1.6 / 7.6	20	80878
8 - 12 / 12 - 16	4.6 / 7.5	20	80879

# Lab assistants

## 2-way connectors, PE-HD

For connecting tubing of varying diameters. The connectors can be joined together with the next size up. Not suitable for pressure applications!


For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3 - 5	1.6	20	80434
5 - 7	2.7	20	80435
7 - 9	3.6	20	80436
9 - 12	5.5	20	80535
11 - 14	7.3	20	80536
13 - 16	8.8	20	80537



## Connectors, T-shape, PP

For the splitting or combining of liquid lines in a tubing system.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3	1.6	20	80459
4 - 5	3.7	20	80460
6 - 7	4.4	20	80461
8 - 9	6.3	20	80462
10 - 11	8.2	20	80463
12 - 13	10.0	20	80520
14 - 15	12.1	20	80521

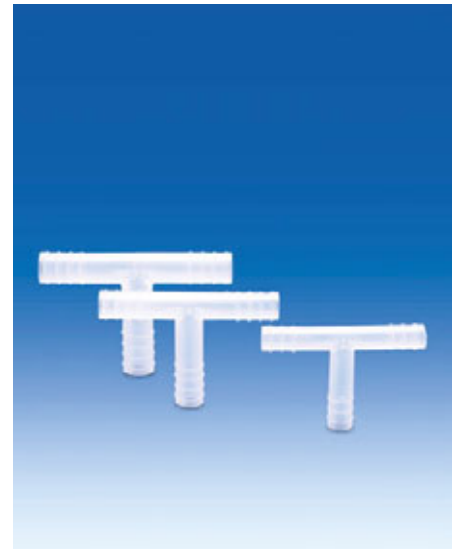

## Connectors, Y-shape, PP

For the splitting or combining of liquid lines in a tubing system.

For tubing with an inner Ø of mm	Outlet opening Ø mm	PU	Cat. No.
3	2.0	20	80464
4 - 5	2.7	20	80465
6 - 7	4.6	20	80466
8 - 9	5.5	20	80467
10 - 11	7.3	20	80468
12 - 13	9.7	20	80525
14 - 15	11.9	20	80526







## Non-return valve, PE-HD

With valve disc made from FKM. Not suitable for pressure applications.

For tubing with an inner $\varnothing$ of mm	PU	Cat. No.
6 - 9	10	78593



## Non-return valves, PP

With valve discs made from EPDM.

The check valve is inserted between the water pump and the vacuum container in the suction line, in order to prevent water backflow when the pressure drops.

Max. operating pressure 2 bar and min. operating pressure 0.07 bar.

For tubing with an inner $\varnothing$ of mm	PU	Cat. No.
8 - 10	10	80418
10 - 15	10	80419



## PTFE-tape

For sealing and wrapping of threads and other connections. High chemical resistance.

Working temperatures up to 250 °C.

Length m	Width mm	PU	Cat. No.
12	12	10	131097



# Lab assistants

## Trays, MF



White. Flat shape. Rounded corners. Smooth surfaces, easy to clean.  
Practical tray for instruments, tools, and sensitive utensils. Stable and self-supporting.

L x W x H mm	PU	Cat. No.
190 x 150 x 17	5	71598
240 x 180 x 17	5	71698
268 x 208 x 17	5	71798
355 x 240 x 17	5	71898
428 x 288 x 17	5	71998



## Trays, MF



White. Tall shape. Rounded corners. Smooth surfaces, easy to clean.  
Practical tray for instruments, tools, and sensitive utensils. Stable and self-supporting.  
Fitting lid made of PS, please order separately.

L x W x H mm	PU	Cat. No.
190 x 150 x 40	5	72098
290 x 160 x 35	5	72198
290 x 160 x 60	5	72398
340 x 245 x 100	5	72498
350 x 250 x 40	5	72298



## Lids for trays, PS

Crystal clear. With handle. Rounded corners. Smooth surfaces, easy to clean.  
Protects the contents of the instrument trays from dust and contamination.  
The contents remain readily visible.

Size mm	For tray, MF No.	PU	Cat. No.
190 x 150	72098	5	79790
290 x 160	72198, 72398	5	79890
340 x 245	72498	5	79990*

\* without handle





## Drawer organiser, PVC

White. With 9 lengthwise compartments opening at the front. For vials with a diameter of 25 mm.

Size mm	Height mm	PU	Cat. No.
355 x 300	45	1	80952



## Drawer organiser, PVC

White. With 12 compartments. Ideal for the orderly storage of small components. Stabilising circumferential edge.

Size mm	Height mm	PU	Cat. No.
410 x 300	65	1	80953



## Drawer organiser, PVC

White. Compartments of 5 different sizes for pipettes, thermometers, connectors, etc. Stabilising circumferential edge.

Size mm	Height mm	PU	Cat. No.
410 x 300	70	1	80954

## Drying rack

Back plate and trough made from PVC with drainage nozzle.

With 75 metal pegs (length: 10 cm) with PE coating for hanging various sizes of apparatus.

With two bore holes for simple wall mounting.

Delivered without installation hardware.

Size mm	PU	Cat. No.
450 x 630	1	76299



## Drying rack, PS

With wide draining trough and drainage nozzles.

Rack with 72 pegs 95 x 15 mm. For drying larger apparatus, some of the pegs can be removed and the bore holes closed at the rear.

Delivered complete with drainage tube and accessories for the wall installation.

In addition, 11 pegs (95 x 6 mm) are included for objects having a smaller diameter, such as reagent tubes.

Description	Size mm	PU	Cat. No.
Drying rack	450 x 630	1	80213
Pegs	95 x 6	11	81213





# VITLAB<sup>®</sup> Promotional

ADVERTISE WITH YOUR GOOD NAME



**VITLAB** <sup>®</sup>  
Competence in Labware

# Your good name in daily use

Precision is usually of great significance when it comes to ensuring the effective use of granulates, powders or liquids. The transportation, storage and decanting of small volumes often require special containers. VITLAB is one of the leading manufacturers of high-grade plastic labware and specializes in high-precision printing on plastic products with superior chemical and break resistance.



This offers a great advantage: by having your name and logo printed on these products, you will work “hand in hand” with your clients and always maintain a high presence. The products can be used wherever people work with granulates, powders or liquids; for example, in agriculture, laboratories, the medical sector, the food industry and the cleaning

business, as well as when using colours and chemicals.

Plastic labware by VITLAB guarantees that you have the best manufacturing quality and optimal functionality associated with your good name, thus ensuring a sustained positive echo.



# A positive echo through individuality

VITLAB develops and manufactures its products at its own production facilities. This allows us to produce and print plastic labware according to your individual requirements and specifications. Please do not hesitate to inform us of your wishes and we will let you know what sort of individual solution we can provide for you.

## When it comes to precision and accuracy


Volumetric containers by VITLAB stand out due to the greater precision and accuracy ensured by the measuring scale. On request, VITLAB can also print a customized scale on your product. The quality colours guarantee that the scale remains readable and does not wear off.

## Small gifts keep the friendship alive

Plastic products have a high level of usability and are ideally suited as advertising articles or for promotional campaigns for your products. You can have your company name and logo or other motifs printed on them permanently and thus advertise with your good name.

## A unique position thanks to an unmistakable design

VITLAB provides advertising materials of the very highest quality with round, conical or flat printing, using screen or pad printing systems and with particularly durable and luminescent colours according to the Pantone and HKS colour table. Various marking techniques, such as laser printing and heat embossing, provide you with an unmistakable design.

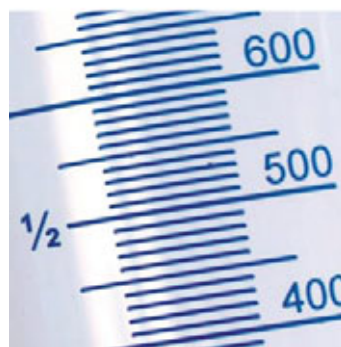



# Would you like to have more information?

---

## Please do not hesitate to contact us!

Please do not hesitate to contact us for advice on the selection, design and colour of your plastic products. A personal consultant ensures that you receive competent advice from the first meeting to the delivery of the product.

Our contact information:

Tel: +49 6026 977 99-0

Fax: +49 6026 977 99 -30

E-mail: [info@vitlab.com](mailto:info@vitlab.com)

[www.vitlab-promotional.com](http://www.vitlab-promotional.com)

# Technical information


---

	Page
• Fluoroplastic PFA	130
• VITLAB <sup>®</sup> opaque	132
• Plastics and their properties	133
• Classification and type description of plastics	133
• Chemical stability of plastics	137
• Physical properties of plastics	146
• Cleaning and maintenance of plastics	147
• Sterilisation of laboratory equipment made of plastics	148
• Disposal and recycling	150
• Suitability for foodstuffs	150
• CE-IVD	151
• Accuracy of volumetric instruments	152


PFA evaporating dish



PTFE beaker

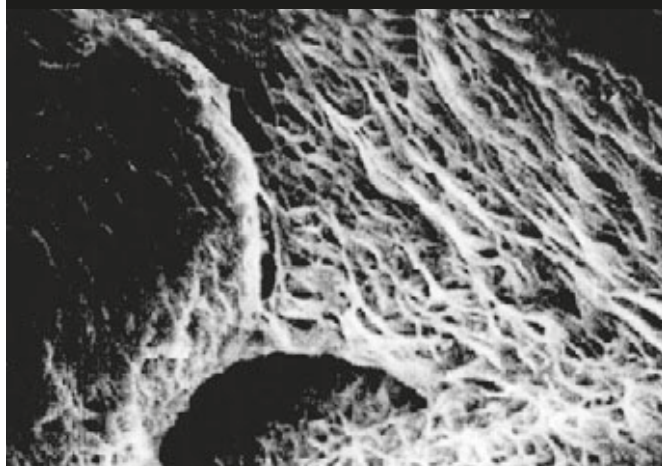

PE-HD bottle

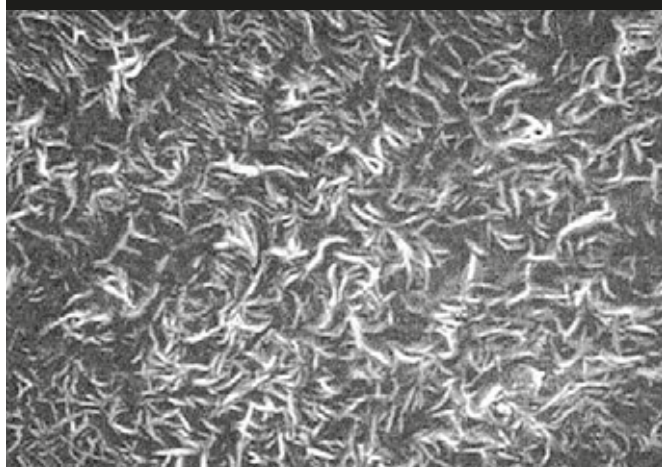

## Fluoroplastic PFA

Today, trace analysis operates with concentrations in the range of ng/g (ppb) and pg/g (ppt). Thus, all modern processes require a corresponding trace analytical laboratory hygiene. However, the analytical accuracy of the measurement depends not only on the accuracy of the analytical instrument, but also directly on the judicious selection of container materials and the preparation of the samples themselves. Under these conditions, the fluoroplastic PFA truly shows its worth.

Labware made from polyolefins, such as polypropylene (PP) or polyethylene (PE), has found broad application in modern laboratories. Since catalysts (e.g., Ziegler-Natta or Philipps) are used during the manufacturing process, the constituent elements (frequently Al, Cr, Mg, Si, Ti or Zn) can still be detected in the ultra-trace range, and thus might affect the analysis results. In direct comparison to these manufacturing processes, PFA is especially suitable for trace element analysis because it is manufactured without the use of additives, and therefore cannot become contaminated by the additive components.

In addition to this advantage, PFA has other remarkable properties. PFA can be used for a broad range of applications by virtue of its resistance to almost all organic and inorganic compounds. PFA is one of the most resistant materials after platinum, and is practically chemically inert. Moreover, PFA stands apart with extraordinarily high thermal stability, making it possible to operate in the temperature range of -200 to +260 °C.

For all PFA products, VITLAB uses only high-purity PFA, which is particularly well-suited for trace analysis. For less critical uses, e.g. if the main requirement is a high chemical resistance, VITLAB offers bottles of "economy grade" PFA, which are partly made of recycled PFA. These are favourably priced and also environmentally friendly.


Pictures of the surface structure of PTFE, PFA, and PE-HD with a scanning electron microscope (8000 times magnification).

# Technical information

VITLAB's PFA vessels have unique, extremely smooth, liquid-repellent surfaces that are made possible through modern manufacturing processes and acknowledged expertise (see pictures on "Surface Structure"). This is especially significant in the illustrative comparison. The pictures taken in a scanning electron microscope show uneven and irregular surfaces for PE-HD and PTFE, and deep pores and concavities can be identified in the PTFE surface. In contrast to the uneven surfaces, PFA evaporating dishes had to be marked (X) and exhibit a completely smooth, even and uniform surface structure.

Due to this characteristic, all PFA labware is particularly easy to clean and presents hardly any interactions with samples as compared to conventional container materials. With these advantages combined with the minimal water absorption by PFA (< 0.03%), even samples at very low concentration can be stored for long periods of time in PFA containers without changes in their concentration (see the application example on Mercury Standards).

Concentration 2 ppb (ng/g) each

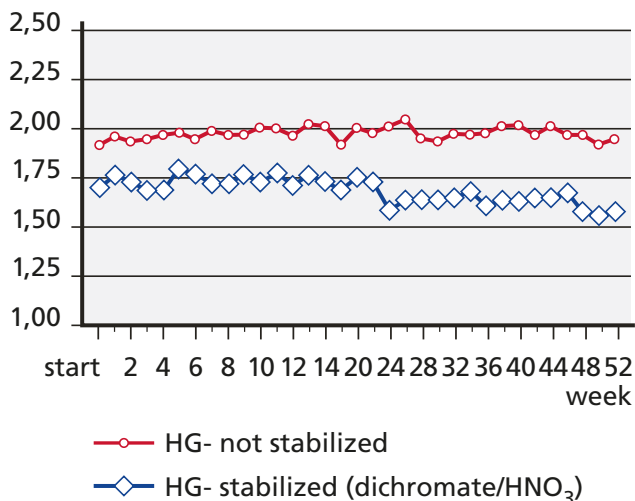


Application Example - Mercury Standards: Storage of an Hg standard in high-purity PFA containers (concentration 2 ppb (ng/g) each). Source: GIT Laboratory Trade Magazine 1/95

## Cleaning after contamination

The valuable properties of PFA, primarily the near absence of memory effects, ensure the reliability of trace analytical results. In comparison with a commercially available glass flask, the simple cleaning after contamination with lead (Pb) solution at a concentration of 1000 ppb (ng/g) is a telling example (see the section on Cleaning of Volumetric Flasks). The cleaning of the glass and PFA volumetric flasks was conducted by shaking with 65% HNO<sub>3</sub> \*Suprapur® (Pb < 0.005 ppm) at room temperature. With PFA volumetric flasks, the minimum concentration of 0.003 ppb is reached after three rinses, while substantially higher lead concentrations can be measured in glass flasks even after four rinses. The experiment also shows that PFA labware does not require the usual time-consuming boiling.

Mean of 4 Graduated Flask 500 ml each

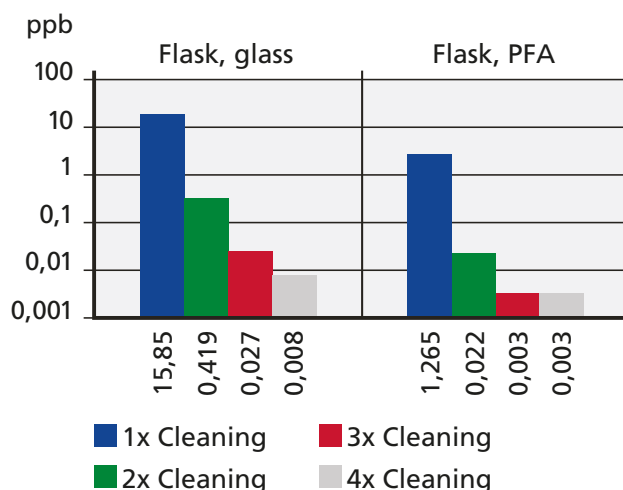

Cleaning of glass and PFA volumetric flasks after contamination. Source: Kali-Forschungsinstitut, K. Mangold

\*Suprapur® is a trademark of Merck KGaA.

## VITLAB® opaque



### Greater protection for light-sensitive substances.

Light-sensitive substances require protection from the effects of light and particularly UV light so that they have a longer usable lifetime. In 2008, VITLAB manufactured the world's first opaque volumetric flasks developed from specially pigmented plastic. The special pigments safely protect samples from the effects of light, while still maintaining high transparency to enable volumes to be set accurately.

The opaque volumetric flasks and reagent bottles safeguard the contained substances with a light protection factor of virtually 20. The absorption spectrum properties exhibited by the products are significantly better over the entire spectral range of 200 - 900 nm versus comparable brown glass products. VITLAB® opaque reagent bottles are especially effective below 560 nm. They have a maximum of 5% transmission at 560 nm, and less than 2.5% transmission measurable at or below 520 nm. The pigments in the opaque products exhibit a brilliant characteristic shine in the UV range starting at 400 nm.

In the UV range from 280 nm and in the upper visible range from 580 nm, VITLAB® opaque reagent bottles and volumetric flasks are thus significantly better than even high-quality brown glass containers. The differences between reagent bottles made of VITLAB® opaque and those of brown glass bottles can be more or less pronounced depending on the type of the glass, since the brown glass bottles are subjected to significantly greater production fluctuations.

The higher break resistance and lower weight are advantageous during daily use in the laboratory, and make VITLAB® opaque an attractive alternative to conventional volumetric flasks and reagent bottles made of brown glass.

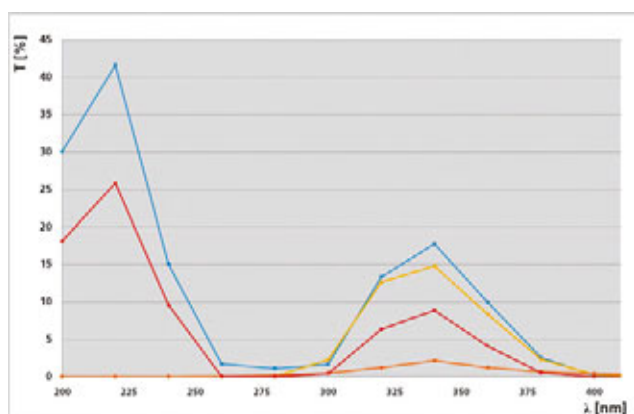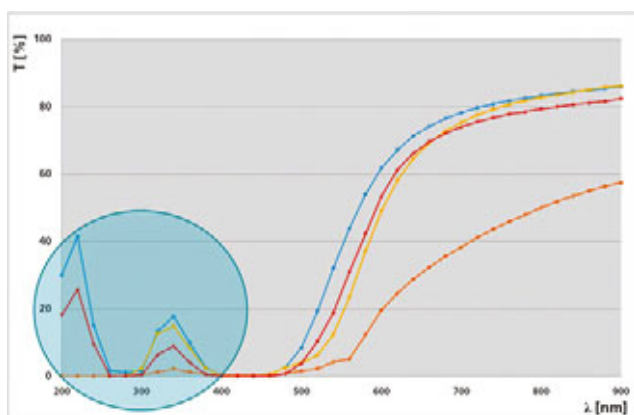

Light transmission diagram: Comparison of results for the measurement of transmission (T%) between VITLAB® opaque and brown glass in volumetric flasks and bottles, in the wavelength range of  $\lambda = 200$  to 900 nm. VITLAB® opaque provides better protection of the container contents from the effects of light, particularly in the UV range (see diagram below).

- Brown glass volumetric flasks
- Brown glass bottle
- ◆— VITLAB® opaque bottle
- ◆— VITLAB® opaque volumetric flask



## Classification and type description of plastics

In general, plastics can be divided into the three groups. The abbreviations of the described plastics used are those according to DIN 7728.


### Thermoplastics

Plastics with a linear molecular structure, with or without side chains, can be reversibly moulded through heat treatment without changing their thermoplastic properties. Thermoplastics are frequently used in the production of plastic labware. Hence we provide here a brief description of some of the more important plastics, and explain their molecular structure, as well as their mechanical, chemical and physical properties. The most frequently used thermoplastics are polyolefins, such as polyethylene and polypropylene.

#### PFA (perfluoroalkoxy copolymer)

121°C


- Highly transparent, elastic thermoplastic with high-molecular, semi-crystalline structure
- Very good temperature stability
- Broad range of application, from -200 °C to +260 °C
- Virtually chemically inert, excellent chemical stability against practically all chemicals
- Very low water absorption (< 0.03%)
- Ultra-smooth, anti-adhesive surface with unique surface structure
- Typical products are, for example: Class A volumetric flasks, bottles, sample containers
  - ➔ Especially suitable for use in trace analysis, and for the storage of low-concentration solutions



#### PTFE Polytetrafluoroethylene

121°C


- Non-transparent, white, elastic thermoplastic with high-molecular, semi-crystalline structure
- Very good temperature stability
- Broad range of application, from -200 °C to +260 °C
- Virtually chemically inert, excellent chemical stability against practically all chemicals
- Anti-adhesive surface
- Very good sliding properties and electrical insulating capability (very low friction coefficient)
- Typical products are, for example: Bottles, beakers, sheathing for magnetic stir bars



#### FEP Tetrafluoroethylene-perfluoropropylene copolymer

121°C


- Translucent, white, thermoplastic copolymer with high-molecular, semi-crystalline structure
- Anti-adhesive surface
- Very good temperature stability
- Broad range of application, from -100 °C to +205 °C
- Excellent chemical stability



#### ETFE Ethylene-tetrafluoroethylene copolymer

121°C


- Translucent, white copolymer from ethylene and tetrafluoroethylene
- Very good temperature stability
- Broad range of application, from -100 °C to +150 °C
- Very good chemical stability
- Typical products are, for example: Thread adapters, Griffin beakers, threaded connectors



#### PMP Polymethylpentene


121°C

- Crystal-clear, stiff thermoplastic
- Similar structure to PP, with the methyl group replaced by an isobutyl group
- Good thermal stability
- Range of application from 0 to +150 °C
- Good tensile strength and dimensional stability
- Good chemical stability
- Typical products are, for example: Class A volumetric flasks, Class A measuring cylinders
  - ➔ For the storage of light-sensitive substances, also available in highly transparent, UV-absorbing VITLAB® opaque






## Classification and type description of plastics



### PP Polypropylene


121°C

- Highly transparent, elastic thermoplastic
- Similar structure to PE, with a methyl group attached to alternate carbon atoms in an isotactic arrangement
- Good thermal stability
- Range of application from 0 °C to +125 °C
- Good tensile strength and dimensional stability
- Good chemical stability, comparable to PE
- Typical products are, for example: Class B volumetric flasks, Class B measuring cylinders, measuring pitchers, sample containers, funnels
  - ➔ For the storage of light-sensitive substances, also available in highly transparent, UV-absorbing VITLAB® opaque




### PE-HD High-density polyethylene

- Transparent, elastic thermoplastic
- Good thermal stability
- Range of application from -50 °C to +105 °C
- Compact, with increased tensile strength due to less cross-linking compared with PE-LD
- Good chemical stability
- Better chemical stability to organic solvents compared to PE-LD
- Typical products are, for example: Bottles, buckets, scoops
  - ➔ For the storage of light-sensitive materials, also available in brown-dyed version



### PE-LD Low-density polyethylene


- Highly transparent, elastic thermoplastic
- Moderate thermal stability
- Range of application from -50 °C to +80 °C
- Very good flexibility
- Good chemical stability
- Typical products are, for example: Wash bottles, dropping pipettes



### PC Polycarbonate

121°C

- Transparent, stiff thermoplastic
- Linear polymer of carbon dioxide
- Very good temperature stability
- Broad range of application, from -130 °C to +125 °C
- Good tensile strength and impact resistance
- Moderate chemical stability
- Typical products are, for example: Desiccators
- Note: Polycarbonates can lose their tensile strength through autoclaving or exposure to alkaline detergents



### POM Polyoxymethylene

121°C

- Non-transparent, white, stiff, and high-molecular thermoplastic
- Good thermal stability
- Broad range of application, from -40 °C to +130 °C
- High hardness and dimensional stability
- Good sliding properties and abrasion resistance
- Good chemical resistance to aliphatic, aromatic, and halogenated hydrocarbons, and alkalis. Unstable to acids and esters
- Typical products are, for example: Slide boxes, staining jars
  - ➔ Especially good chemical stability to organic solvents
  - ➔ POM can replace metal in many applications




# Technical information

## Classification and type description of plastics


### PA Polyamide

- Linear polymers with regularly repeating amide bonds along the main chain
- Good thermal stability
- Range of application from -40 °C to +100 °C
- Outstanding durability and tensile strength, often used as construction material and for metal coatings
- Good chemical resistance to organic solvents
- Readily attacked by acids and oxidising agents
- Typical products are, for example: Spatula




### SAN Styrene-acrylonitrile copolymer

- Crystal clear, stiff thermoplastic copolymer
- Moderate thermal stability
- Range of application from -40 °C to +70 °C
- Brittle and dimensionally stable
- Low tendency to form stress cracks
- Moderate chemical stability, SAN is slightly more chemically stable than PS
- Typical products are, for example: Graduated beakers, Class B graduated cylinders




### PMMA Poly(methyl methacrylate)

- Crystal clear ("organic glass"), dimensionally stable thermoplastic
- Moderate thermal stability
- Range of application from -50 °C to +65 °C
- Very good UV radiation stability
- Poor chemical stability
- Typical products are, for example: Cuvettes




### PS Polystyrene

- Crystal clear, stiff, amorphous or semi-crystalline thermoplastic
- Moderate thermal stability
- Range of application from -20 °C to +70 °C
- Hard, brittle, and dimensionally stable
- Tendency to form stress cracks
- Moderate chemical stability
- Typical products are, for example: Containers, cuvettes



### PVC Poly(vinyl chloride)


- Amorphous thermoplastic, transparent with a slight blue tint
- Moderate thermal stability
- Range of application from -20 °C to +80 °C
- Good chemical stability, especially resistant to oils
- The addition of plasticisers opens up many useful applications, ranging from artificial leather to injection moulding components
- Typical products are, for example: Drawer organisers, dishes, trays



## Classification and type description of plastics

### Thermosets

Plastics with densely cross-linked molecules, which are very hard and brittle at normal temperatures. Heating causes irreversible hardening. These plastics are rarely used for plastic labware. The best known thermosets are the melamine resins. Melamine resin is produced by polycondensation of melamine with formaldehyde.




#### MF Melamine-formaldehyde resin

- Colourless thermoset, also belongs to the aminoplast group
- Good thermal stability
- Broad range of application, from -80 °C to +120 °C
- High surface hardness, abrasion resistance, and fire resistance
- Good electrical insulator, high creep resistance
- Good chemical stability
- Typical products are, for example: Trays, plates, mixing bowls
- Caution necessary when used in a microwave oven: Heating can release amounts of melamine and formaldehyde that can be harmful to health!


### Elastomers

Plastics with loosely cross-linked molecules that exhibit rubber-like elasticity at room temperature. Heating causes irreversible integration (vulcanisation). The best known elastomers are natural rubber and silicone rubber.




#### NR Natural rubber

- Elastomer obtained from latex (milk-like sap from rubber tree bark) and vulcanised with sulphur to improve the elasticity
- Composed of polymerised isoprene, with an extremely uniform structure
- Moderate thermal stability, not stable to UV
- Range of application from -40 °C to +80°C
- High tensile strength and elongation at rupture
- Poor chemical stability
- Typical products are, for example: pipette filler bulbs



#### SI Silicone rubber

- Synthetic elastomer in which silicon atoms are linked together by oxygen atoms
- Includes polyorganosilanes that have groups such as hydrogen atoms, hydroxyl groups or vinyl groups for cross-linking reactions
- Very good thermal stability, and resistance to UV, ozone, and weather
- Broad range of application, from -60 °C to +180 °C
- High dimensional stability, even at high temperatures
- Very good durability, even at low temperatures
- Poor chemical stability



#### EPDM Ethylene-propylene-diene rubber

- Synthetic terpolymeric elastomer
- Manufactured with metallocene or Ziegler-Natta catalysts that utilise vanadium compounds and aluminium alkyl chlorides
- Good thermal stability
- Range of application from -40 °C to +130 °C
- High elasticity, even at low temperatures
- Stable to UV and ozone, and weather-resistant
- Very good chemical stability

# Technical information

## Chemical resistance of plastics

With regard to chemical stability, plastics are classified as follows:

<p style="font-size: 2em; font-weight: bold;">+</p> <p style="font-weight: bold;">Very good chemical resistance</p> <p>Within 30 days, continuous exposure to media causes no damage to the plastic. The plastic may remain resistant for years.</p>	<p style="font-size: 2em; font-weight: bold;">0</p> <p style="font-weight: bold;">Good to limited chemical resistance</p> <p>Within 7-30 days, continuous exposure to media causes minor damage (e.g. swelling, softening, loss of mechanical strength, discolouration), some of which is reversible.</p>	<p style="font-size: 2em; font-weight: bold;">-</p> <p style="font-weight: bold;">Poor chemical resistance</p> <p>Not suitable for continuous exposure to media. Immediate damage may occur (e.g. loss of mechanical strength, deformation, discolouration, cracking, liquification).</p>
--	---	---

## Chemical resistance of plastics to various substance classes

Classes of substances at 20 °C	PFA	PTFE	FEP	ETFE	PMP	PP	PE-HD	PE-LD	PC	POM	PA	SAN	PMMA	PS	PVC	MF	NR	SI	EPDM	FKM
Alcohols, aliphatics	+	+	+	+	+	+	+	+	+	+	0	+	-	+	+	+	+	+	+	-
Ethers	+	+	+	+	-	0	0	0	-	+	+	-	-	-	-	-	-	-	-	-
Aldehydes	+	+	+	+	0	+	+	0	0	0	0	-	0	-	-	+	0	0	+	+
Esters	+	+	+	+	0	0	0	0	-	-	+	-	0	-	-	+	0	0	0	-
Hydrocarbons, aliphatic	+	+	+	+	0	+	+	0	0	+	0	-	+	-	+	+	-	-	-	0
Hydrocarbons, aromatic	+	+	+	+	-	0	+	0	-	+	0	-	-	-	-	+	-	-	-	0
Hydrocarbons, halogenated	+	+	+	+	-	0	0	0	-	+	0	-	-	-	-	+	-	-	-	0
Ketones	+	+	+	0	0	0	0	0	-	+	+	-	-	-	-	+	-	-	0	-
Alkalis	+	+	+	+	+	+	+	+	-	+	+	+	+	+	+	-	+	0	+	0
Acids, strong or concentrated	+	+	+	+	+	+	+	+	-	-	-	-	-	0	+	-	-	-	+	0
Acids, weak or diluted	+	+	+	+	+	+	+	+	0	-	-	0	-	0	+	0	0	0	+	+
Oxidising acids, oxidising agents	+	+	+	+	-	-	-	-	-	-	-	-	-	-	-	-	-	-	0	0

The carefully prepared recommendations listed here are based on technical literature and made available by the manufacturers of raw materials, to provide information and advice. However, nothing can replace suitability tests conducted by the end user under the actual conditions of use.

## Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Acetaldehyde	+	+	+	+	+	0	0	-	+	-	+	0	+	-
Acetic acid (glacial acetic acid), 100%	+	+	+	+	+	+	+	0	+	0	+	+	+	0
Acetic acid, 50%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Acetic anhydride	+	+	+	+	+	+	+	0	0	0	0	0	-	-
Acetone	+	+	+	+	+	0	+	+	+	+	+	+	+	0
Acetonitrile	+	+	+	+	+	+	0	-	+	0	+	0	+	0
Acetophenone	+	+	+	+	+	+	0	-	0	0	0	0	-	-
Acetyl chloride(acetic acid chloride)	+	+	+	+	+	+			+		+		+	
Acetylacetone	+	+	+	+	+	+	+		+		+		+	
Acrylic acid (2-propenic acid)	+	+	+	+	+	+	+		+		+		+	
Acrylonitrile	+	+	+	+	+	+	-	-	0	-	+	+	+	+
Adipic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Allyl alcohol (2-propan-1-ol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Aluminium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Aluminium hydroxide	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Amino acids	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium fluoride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium hydroxide, 30% (ammonia)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ammonium sulphate			+	+			+	+	+	+	+	+	+	+
n-Amyl acetate (pentyl acetate)	+	+	+	+	+	+	+	0	0	-	+	0	0	-
Amyl alcohol (pentanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Amyl chloride (chloropentane)	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Aniline	+	+	+	+	+	0	+	0	+	+	+	+	+	0
Aqua regia	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Barium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Benzaldehyde	+	0	+	+	+	0	+	+	+	+	+	+	+	+
Benzene	+	+	+	+	+	+	0	0	+	0	+	+	0	-
Benzoyl chloride			+	+	+	+	0	0	+	0	+	+	0	-
Benzyl alcohol	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Benzyl chloride			+	+	+	+								
Benzylamine	+	+	+	+	+	+	0		0		0		0	-
Boric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Bromine	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Bromobenzene	+	+	+	+	0	-	-	-	-	-	-	-	-	-
Bromoform	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Bromonaphthalene	+	+	+	+	+	+								
Butanediol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
1-Butanol (butyl alcohol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
n-Butyl acetate (acetic acid n-butyl ester)	+	+	+	+	+	+	+	0	0	0	+	+	0	0
Butyl methyl ether	+	+	+	+	+	0	+	-	+	0	0	-	0	-
Butylamine			+	+	+	+								
Butyric acid (butanoic acid)	+	+	+	+	+	+			-	-	0	-	-	-
Calcium carbonate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Calcium hypochlorite	+	+	+	+	+	+	+	0	+	+	+	+	+	+

# Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	20 °C	20 °C	20 °C	20 °C
0	-	+	+	0		-	-	-	-	-	-	-	-		-	-	0	-
-	-	-	-	-	-					-	-			0	0	0	0	-
+	0	0	-	-	-	+	0	-	-	0	0	+	0	+	-	-	-	-
-	-	-	-	0	0					-	-	-	-		0	0	0	-
-	-	+	+	+		-	-	-	-	-	-	-	-	+	0	-	+	-
-	-	+		+		-	-	-	-	-	-	-	-		-	-	-	-
-	-	+		+		-	-	-	-	-	-	-	-	+	-	-	+	-
-	-			-	-	-	-	-	-	-	-	-	-		-	-	-	+
-	-	+				-	-	-	-	-	-	-	-		-	-	+	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	-
+	+	+	+	+		+	+	+	+	+	+	+	0		+	+	+	+
0	0	+	+	0		0	-	-	-	0	0	0	-		0	-	+	+
-	-	+	0	0	-	+	+	+	+	+	+	+	0	+	0	0	+	+
0	-	+	+	+	+	0	0	0	0	0	0	+	+		+	+	+	+
+	+	+	+	+	+	+	+	+	+	+	+	+	+		+	+	+	+
0	0	+	+	+		+	+	0	0	+	+	+	0		+	+	+	+
0	0	+	+	+		+	+	0	0	+	+	+	0		-	+	+	0
-	-	0	0	0		+	0	+	+	0	-	+	0	+	+	0	+	-
+	+	+	+	+		+	+	+	+	+	+	+	+		0	0	+	-
-	-	+	+	0		-	-	+	+	-	-	-	-		0	-	0	-
+	+	+	+	+		+	+			0	0	0	0		0	-	0	0
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	+
0	-	0	0	0	-	-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
0	-	+	+	0		-	-	-	-	-	-	-	-		-	-	0	-
-	-	+	0	+		-	-	-	-	-	-	-	-	+	-	-	-	0
-	-	+	0	-	-	-	-	-	-	-	-	-	-		-	-	-	+
0	0	+	+	-	-	-	-	-	-	-	-	0	0		-	0	0	+
		+		+		-	-	-	-	-	-				-	-	-	+
-	-	+				-	-	-	-	-	-	-	-		-	0	0	+
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	0
-	-			+		-	-	-	-	-	-	-	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-		
		+	+	+		-	-	-	-	-	-				0	-	+	-
0	0	+	+	+	0	+	0	0	-	0	-	0	0		+	0	0	+
-	-	+	0	+		-	-	-	-	-	-	-	-		-	-	0	-
-	-	+	+			-	-	-	-	-	-	-	-		-	-	-	-
		+	+			-	-	-	-	-	-				-	0	-	-
0	-			0	0	-	-			-	-				-	-	-	0
+	+	+	+	+	+	+	+	+	+	+	+	+	+		+	+	+	+
+	+	+	+	-	-	+	+	+	+	+	+	0	-		+	+	+	+
-	-	+	+	+		+	0	+	+	+	0	+	+		+	0	+	+
0	-	+	+	+	-	+	+	0	0	+	+	0	-		-	0	+	+

## Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Carbon disulphide	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Carbon tetrachloride	+	+	+	+	+	+	-	-	-	-	0	-	0	-
Chloroacetaldehyde, 45%			+	+	+	+								
Chloroacetic acid (monochloroacetic acid)	+	+	+	+	+	+	+	0	+	0	+	+	+	+
Chloroacetone			+	+	+	+								
Chlorobenzene	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Chlorobutane	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Chloroform	+	0	+	+	+	0	0	-	-	-	0	-	0	-
Chloronaphthalene			+	+	+	+								
Chlorosulphonic acid	+	+	+	+	0	-								
Chromic acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Chromic acid, 50%	+	+	+	+	+	+	0	0	0	0	+	0	+	0
Chromic-sulphuric acid	+	+	+	+	+	+	0	-	-	-	-	-	-	-
Copper sulphate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Cresol	+	+	+	+	+	0	-	-	0	0	0	-	-	-
Cumene (isopropylbenzene)	+	+	+	+	+	+	-	-	0	-	+	0	0	-
Cyclohexane	+	+	+	+	+	0	-	-	0	-	0	-	0	-
Cyclohexanone	+	+	+	+	+	+	0	0	0	-	0	-	-	-
Cyclopentane	+	+	+	+	+	+	0	-	0	-	0	-	-	-
Decane	+	+	+	+	+	+	0		0		0	-		
1-Decanol	+	+	+	+	+	+	+		+		+			
Di(ethylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Dibenzyl ether	+	+	+	+	+	+	0		+		+			
Dibromoethane	+		+	+	0									
Dibutyl phthalate	+	+	+	+	+	+	+	0	+	0	0	-	0	-
Dichloroacetic acid	+	+	+	+	+	0	+	+	0	-	0	0	0	-
Dichlorobenzene	+	+	+	+	+	0	-	-	0	-	0	-	0	-
Dichloroethane	+	+	+	+	+	+	0	-	0	-	0	-	0	-
Dichloromethane (methylene chloride)	+	+	+	+	0	0	0	-	0	-	0	-	0	-
Diesel oil (heating oil)	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Diethanolamine			+	+					0		0			
Diethyl ether	+	+	+	+	+	+	-	-	0	-	0	-	-	-
Diethylamine	+	+	+	+	+	0	0	0	0	-	0	-	-	-
1,2 Diethylbenzene	+	+	+	+	+	0	-	-	-	-	0	-	-	-
Dimethyl sulphoxide (DMSO)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Dimethylaniline	+	+	+	+	+	+								
Dimethylformamide (DMF)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
1,4-Dioxane	+	+	+	+	+	0	0	0	+	0	+	+	+	0
Diphenyl ether			+	+										
1,2 Ethanediol (ethylene glycol, glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ethanol (ethyl alcohol)	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Ethanolamine	+	+	+	+	+	+			+					
Ethyl acetate (acetic acid ethyl ester)	+	+	+	+	+	+	0	-	+	0	+	+	+	+
Ethyl methyl ketone (MEK)	+	+	+	+	0	0	-	-	+	0	0	-	0	-
Ethylbenzene	+	+	+	+	0	0	-	-	-	-	-	-	-	-
Ethylene oxide	+	+	+	+	+	+	0	-	0	-	0	0	0	0
Fluoroacetic acid			+											

# Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	20 °C	20 °C	20 °C	20 °C
-	-	+	+	0		-	-	-	-	-	-	-	-		-	-	-	+
-	-	0	0	-	-	-	-	0	-	-	-	-	-	+	-	-	-	+
0	-	-	-	-	-	-	-	0	-	0	-	+	0		-	-	0	0
															0	-	+	-
-	-			-	-	-	-	-	-	-	-	-	-		-	-	-	0
-	-	-	-	0	-	-	-	-	-	-	-	-	-	+	-	-	-	0
+	0	0	0	-	-	-	-	0	-	-	-	+	0		-	0	-	+
0	-	-	-	-	-	0	0	-	-	-	-	+	-		-	-	-	+
-	-	-	-	-	-	0	0	-	-	0	0	+	0		-	-	-	+
+	+	+	+	+		+	0	+	+	+	+	+	0		0	+	+	+
-	-			-	-										-	-	-	+
-	-	+	-			-	-	-	-	-	-	-	-		-	-	-	+
-	-	+	+	+										+	-	-	-	+
-	-			+											-	-	-	-
-	-														-	-	-	+
0		+										0			-	0	-	+
0		+				0				0		+			0	0	+	+
0	0	+	0	0		+	+	-	-	0	-	-	-		+	0	+	+
		+				-	-	-	-	-	-				-	-	0	-
-	-	+	+			-	-	-	-	-	-	-	-		-	0	0	0
0	-			-	-					0	-	0	-		-	-	-	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	+
				0														
-	-	-	-	0	-					-	-	-	-		-	-	-	0
-	-	+	+	+	+	-	-	0	-	-	-	0	-		-	-	-	+
-	-					-	-	-	-	-	-						0	
-	-									0	0	-	-		0	0	0	-
0	-									-	-	-	-		-	-	-	+
-	-					-	-	-	-	-	-	-	-		+			
-	-					-	-	-	-	-	-	-	-		-	0	0	0
-	-	+	+	+		-	-	-	-	-	-	0	-		0	0	0	-
0	0	0	0	+		-	-	-	-	-	-	-	-		-	-	0	-
		0		0		-	-	-	-	-	-				-	-	-	0
+	+	+	+	0	0	+	+	+	+	+	+	+	+	+	-	+	+	0
+	0	+	+	+		0	-	-	-	0	-	+	0	+	0	0	+	0
																	+	
-	-			+						-	-	-	-	+	-	-	0	-
-	-	-	-	+		-	-	-	-	-	-	-	-		-	-	-	-
-	-					-	-	-	-	-	-	-	-		-	-	-	0
0	-	+	+	0		-	-	-	-	-	-	0	-		-	-	-	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	-	-



## Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Formaldehyde, 40%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Formamide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Formic acid, 98-100%	+	+	+	+	+	+	+	0	+	+	+	+	+	+
Gasoline (petroleum spirits)	+	+	+	+	+	+	0	0	0	0	+	+	0	-
Glycerine	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Glycolic acid, 70%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Heating oil (Diesel oil)	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Heptane	+	+	+	+	+	+	0	0	0	0	0	0	0	-
Hexane	+	+	+	+	+	+	0	-	+	0	+	0	0	-
Hexanoic acid			+	+										
Hexanol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 20%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrochloric acid, 37%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrofluoric acid, 40%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrofluoric acid, 70%	+	+	+	0	+	+	+	0	+	0	+	0	+	-
Hydrogen bromide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydrogen peroxide, 35%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Hydroiodic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isoamyl alcohol (3-methyl-1-butanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isobutanol (isobutyl alcohol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isooctane	+	+	+	+	+	+								
Isopropanol (2-propanol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Isopropyl ether	+	+	+	+	+	0	-	-	-	-	-	-	-	-
Lactic acid (2-hydroxypropionic acid)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Lugol's solution (iodine/potassium iodide solution)	+	+	+	+	+	+	+	0	+	+	-	-	-	-
Mercury	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Mercury chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Methanol	+	+	+	+	+	+	+	+	+	+	+	+	+	0
Methoxybenzene	+	+	+	+	+	+								
Methyl butyl ether	+	+	+	+	+	0	+	0	+	+	0	-	-	-
Methyl ethyl ketone (MEK)	+	+	+	+	0	0	-	-	+	0	0	-	0	-
Methyl formate (formic acid methyl ester)	+	+	+	+	+	+								
Methyl propyl ketone	+	+	+	+	+	+	0	0	+	0	+	+	+	0
Methylene chloride (dichloromethane)	+	+	+	+	+	+	-	-	0	-	0	-	0	-
Mineral oil (motor oil)	+	+	+	+	+	+	+	+	+	+	+	+	+	0
Monochloroacetic acid	+	+	+	+	+	+	+	0	+	0	+	+	+	+
Nitric acid, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Nitric acid, 30%	+	+	+	+	+	+	0	-	0	-	0	-	0	0
Nitric acid, 70%	+	+	+	+	+	+	-	-	-	-	-	-	-	-
Nitrobenzene	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Oleic acid	+	+	+	+	+	+								
Oxalic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Ozone	+	+	+	+	+	+	+	+	0	-	0	-	0	-
n-Pentane	+	+	+	+	+	+								
Peracetic acid	+	+	+	+	+	+								
Perchloric acid	+	0	+	+	+	+	0	-	+	-	+	-	+	-
Perchloroethylene	+	+	+	+	+	+	-	-	-	-	-	-	-	-

# Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	20 °C	20 °C	20 °C	20 °C
+	0	+	+	+	0	+	+	-	-	-	-	0	-		0	0	+	0
		-	-	+											+		0	0
+	0	-	-	-	-	0	0	-	-	+	0	-	-	+	0	-	0	-
0	-	+	+	+		-	-	+		-	-	0	-	+	-	-	-	+
+	+	0	0	+	+	+	+	+	+	+	+	+	+	+	0	+	+	0
				-	-										+	+	+	0
-	-	+	+	+		-	-	0	-	-	-	0	-		-	-	-	+
+	0			+				0	-	-	-	-	-		-	-	-	+
-	-	+	+	+		+	+	0	0	-	-	0	-		-	-	-	+
								+										
								+							0	0	-	+
-	-	-	-	-	-	0	-	0	-	+	+	+		-	0	0	+	+
0	0	-	-	-	-	0	-	0	-	+	+	0		-	0	-	+	+
-	-	-	-	-	-	0	-	0	-	0	0	0	-	-	0	-	+	0
-	-	-	-	-	-	+	0	-	-	+	+	0	-	-	-	-	0	0
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
+	+	-	-	-	-					0	-				0	-	0	+
+	+	+	-	-	-	+	+	-	-	+	+	+	0	0	-	0	0	
																	+	+
		+	+												0	0	0	0
+	+	+	+			0	-	0	-	0	0	+	0		+	+	+	+
0				+		0	-			0	-				-	-	-	+
+	+	+	+	+		+	-	0	-	0	0	+	0		+	0	+	+
-	-			-	-					-	-	-	-		-	-	-	-
+	+	+	-	0	-	+	+	0	-	+	+	0	0		0	0	0	+
0	-	0	0			0	-	-	-	0	-	-	-		+	-	+	+
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
+	+	0	0	-	-	+	+	+	+	+	0	-	-		+	+	+	+
+	0	+	+	0		0	-	-	-	0	-	+	0		0	+	+	-
-	-	0				-	-	-	-	-	-				-	-	-	-
-	-	0				-	-	-	-	-	-	-	-		-	-	-	-
-	-	-	-			-	-	-	-	-	-	-	-		-	-	0	-
-	-	+				-	-	-	-	-	-				-	0	0	
-	-	+	+			-	-	-	-	-	-	-	-		-	-	0	-
-	-	-	-	0	-	-	-	-	-	-	-	-	-		-	-	-	0
+		+	+			+		+	+	+		+	+		-	0	-	+
0	-	-	-	-	-	-	-	0	-	0	-	+	0		-	-		0
+	0	-	-	-	-	+	0	+	0	-	-	+	0	-	-	-	0	0
+	0	-	-	-	-	0	-	0	0	-	-	0	-	-	-	-	-	0
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
-	-	0	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
				+		-	-	-	-	-	-				-	-	-	0
+	+	+	+	-	-	+	+	+	+	+	+	+	+		0	0	+	+
-	-	-	-	-	-	0	0	+	0	0	0	+	0		-	+	+	+
				+											-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	0	-		-	-	0	+
-	-	+	0	-	-	0	0	0	-	-	-	-	-		-	-	-	0

## Chemical stability of plastics

Medium	PFA/FEP		PTFE		ETFE		PMP		PP		HDPE		LDPE	
	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C
Petroleum	+	+	+	+	+	+	0	0	0	-	0	-	0	-
Petroleum ether	+	+	+	+	+	+							0	
Phenol	+	+	+	+	+	+	0	0	+	+	+	+	+	0
Phenylethanol	+	+	+	+	+	+			0		0			
Phenylhydrazine	+	+	+	+	+	+			0		0			
Phosphoric acid, 85%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Piperidine	+	+	+	+	+	+			+		+			
Potassium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Potassium dichromate			+	+										
Potassium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Potassium permanganate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Propanol	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Propionic acid	+	+	+	+	+	0	+	0	+	0	+	0	0	-
Propylene glycol (propanediol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Pyridine	+	+	+	+	-	-	+	0	0	0	+	0	+	0
Salicylaldehyde	+	+	+	+	+	-	+	+	+	+	+	+	+	+
Salicylic acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Silver acetate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Silver nitrate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium acetate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium chloride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium dichromate	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium fluoride	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sodium hydroxide	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sulphuric acid, 60%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Sulphuric acid, 98%	+	+	+	+	+	+	+	+	-	-	0	-	0	-
Tartaric acid	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Tetrachloroethylene	+		+	+	0									
Tetrahydrofuran (THF)	0	0	+	+	+	0	0	-	-	-	0	-	0	-
Tetramethylammonium hydroxide	+	+	+	+	+	+								
Toluene	+	+	+	+	+	+	0	-	0	-	0	0	0	-
Tri(ethylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Tri(propylene glycol)	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Trichloroacetic acid	+	+	+	+	+	0	+	+	0	-	0	0	0	-
Trichlorobenzene	+	+	+	+	+	0	0	0	-	-	-	-	-	-
Trichloroethane	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Trichloroethylene	+	+	+	+	+	+	-	-	-	-	0	-	-	-
Trichlorotrifluoroethane	+	+	+	+	0	-								
Triethanolamine	+	+	+	+										
Trifluoroacetic acid (TFA)	+	-	+	0										
Trifluoroethane	+	0	+	+										
Turpentine	+	+	+	+	+	+	0	0	-	-	0	-	0	-
Urea	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Xylene	+	+	+	+	+	+	0	-	-	-	0	-	0	-
Zinc chloride, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+
Zinc sulphate, 10%	+	+	+	+	+	+	+	+	+	+	+	+	+	+

# Technical information

PC		POM		PA		SAN		PMMA		PS		PVC		MF	NR	SI	EPDM	FKM
20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	50 °C	20 °C	20 °C	20 °C	20 °C	20 °C
0	0	+	+	+				+		-	-	+	-		-	0	-	+
		+	+	+				+		-	-	0	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	0
				0											0	-	-	0
+	+	+	-	-	-	+	+	-	-	+	0	+	0	-	-	-	0	+
															-	-	-	-
+	+	+	+	+		0	0	+	+	0	0	+	0		+	+	+	+
				-	-										0	0	+	0
-	-	+	+	+		0	0	+	+	0	0	0	0	-	0	-	+	-
+	+	0	0	-	-	+	0	+	+	+	+	+	+		-	-	+	+
0		+	+	+	+	+	+	0		0		+	+		+	0	+	+
-	-	-	-	0	0					0	-	0	-		-	-	0	+
+	0	+	+	-	-	-	-	0	0	+	+	0	-		+	+	+	+
-	-	+	0	+		-	-	-	-	-	-	0	-		-	-	-	-
0	0					-	-			-	-	-	-					
		-	-	+		+	+			+	+	0	-		+	+	+	+
+	+	0	0			0	0	0	0	0	0	0	0		+	+	+	+
+	+	0	0	+		+	+	+	+	0	0	0	0		+	+	+	+
+	+	+	0	+		+	+	-	-	+	+	0	0		+	0	+	-
+	+	+	+	+		+	+	+	+	+	+	+	+		+	+	+	+
+	-	+	+	+		+	0	+	0	+	0	+	+		+	0	+	+
+	+	+	+	+		+	+	+	+	+	+	+	+		0	0	+	+
-	-	+	+	+	0	+	+			+	+	+	+	-	0	0	+	0
0	0	-	-	-	-	+	0	-	-	-	-	0	-		-	-	-	+
-	-	-	-	-	-	-	-	-	-	-	-	-	-		-	-	-	+
+	+	+	+	0	0	+	+	0	0	+	+	+	+	-	+	+	0	+
				-	-										-	-	-	0
-	-	0	0	+		-	-	-	-	-	-	-	-	+	-	-	-	-
-	-	-	-														+	-
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	0
+	0	+	0			+	+	0	0	+	+	0	-		0	+	+	+
+	0	+	0			+	+	0	0	+	+	0	-		+	+		
0	-			-	-					0	-	0	-		0		0	-
-	-									-	-	-	-					
-	-	0	-	0		-	-	-	-	-	-	-	-		-	-	-	+
-	-	-	-	0		-	-	-	-	-	-	-	-		-	-	-	0
				0		-	-			-	-						0	
						-	-			-	-				0	-	0	-
		-	-			-	-			-	-							-
						-	-			-	-				-	-	-	+
-	-	+	+	+		0	0	+	+	-	-	+	+		-	-	-	+
-	-	+	+	+		+	+	+	+	+	+	0	-	+	+	+	+	+
-	-	+	+	+		-	-	-	-	-	-	-	-		-	-	-	0
+	+	+	0	-	-	+	+	-	-	+	+	+	0		+	+	+	+
+	+	0	-	-	-	+	+	0	0	+	+	+	0		0	+	+	+

## Physical properties of plastics

Plastics	Max. temperature for use °C	Brittleness temperature °C	Microwaveability*	Density g/cm <sup>3</sup>
PFA	260	-200	yes	2,17
PTFE	260	-200	yes	2,17
FEP	205	-100	yes	2,15
ETFE	150	-100	yes	1,70
PMP	150	0	yes	0,83
PP	125	0	yes	0,90
PE-HD	105	-50	yes	0,95
PE-LD	80	-50	yes	0,92
PC	125	-130	yes	1,20
POM	130	-40	no	1,42
PA	90	0	-	1,13
SAN	70	-40	no	1,03
PMMA	65 - 95	-50	no	1,18
PS	70	-20	no	1,05
PVC	80	-20	no	1,35
MF	120	-80	yes**	1,50
NR	80	-40	no	1,20
SI	180	-60	no	1,10
EPDM	130	-40	-	-
FKM	220	-30	-	-

\* Mind the chemical and temperature suitability!

\*\* Caution necessary when used in a microwave oven: Heating can release amounts of melamine and formaldehyde that can be harmful to health!

## Cleaning and maintenance of plastics

---

All polyolefins, such as PE-LD, PE-HD, PP and PMP, as well as the fluoroplastics PTFE, PFA, FEP and ETFE have water-repellent surfaces that are very durable and easy to clean. For cleaning, depending on the level of contamination, commercially available neutral or alkaline detergents can be used. Polycarbonate (PC) labware should not be cleaned with alkaline cleaning agents (> pH 7). Please note that no scrubbing agents or scouring pads should be used for labware made from plastics.

### **Cleaning with dishwashers**

Labware made from the above-named plastics (except for PE-LD, due to the temperature limit) can be cleaned and dried in a laboratory dishwasher together with other apparatus. Machine cleaning with laboratory dishwashers is gentler to labware than cleaning in an immersion bath. The labware is exposed to the cleaning solution for relatively short rinsing periods when sprayed by the jet or injector nozzles. Due to their light weight, we recommend securing the apparatus to be washed with washing nets to prevent them from tumbling in the water jet. Labware is better protected against scratching when the wire baskets in the washing machine are plastic coated.

### **Cleaning in an ultrasonic bath**

Plastic labware may be cleaned in an ultrasonic bath. However, direct contact with the acoustic membrane should be avoided.

### **Cleaning in trace analysis**

To avoid contamination with cations and anions in trace analysis, plastic labware should be allowed to stand with a 1N HCl or HNO<sub>3</sub> solution for a maximum of 6 hours at room temperature, and be rinsed afterwards with purified distilled water. For trace analysis conducted in the concentration range of ng/g (ppb) or pg/g (ppt), containers made of the fluoroplastic PFA are particularly suitable, because they have a smooth surface, are easy to clean without carry-over (memory effects) and interaction with the container material.

## Sterilisation of laboratory equipment made of plastics

### Autoclaving

#### Recommended autoclaving protocol

20 minutes at 121 °C (2 bar),  
according to DIN EN 285

Autoclaving (steam sterilisation) is defined as the destruction or irreversible inactivation of all reproducible microorganisms under exposure to "saturated steam at a minimum of 120 °C." (DIN 58946-1, 1987). DIN EN 285 specifies a minimum exposure time ( $t_g$ ) of 20 minutes (killing time and safety margin) at a sterilisation temperature of 121 °C. For the correct sterilisation procedure, including biological safety (DIN EN 285), please contact your hygiene specialist.

Prior to autoclaving plastic labware, ensure that no soiling or residual contamination remains on the equipment. Otherwise, the residual contamination will bake on solidly during the autoclaving process. Even substances that have no effect on the plastic at room temperature can still lead to destruction of the plastic during the autoclaving process. Additionally, microorganisms might not be killed effectively if they are protected by the residual contamination.

### Notes on autoclaving



- Containers with screw tops or stoppers must be **open** during autoclaving to allow for pressure equalisation
  - ➔ Autoclaving of a closed container will lead to the deformation or destruction of the container
- Plastic labware should be **stood upright on a level surface** during autoclaving to avoid shape deformation.
  - ➔ Plastic labware should not be laid on its side during autoclaving
- **No mechanical stresses** should be present during autoclaving
  - ➔ For example, do not stack items
- Do not autoclave any container that contains residual contamination or even rinsing agent
- Not all plastics are resistant to steam sterilisation! For example, polycarbonate loses its tensile strength
  - ➔ Mind the temperature limits for the plastics
  - ➔ Autoclavable products are identified with a "121 °C" symbol in this catalogue

The surfaces of some plastics can be attacked by chemicals present during autoclaving, which can cause persistent clouding. Some transparent plastics can absorb minute quantities of steam, which can lead to reversible clouding. This clouding disappears upon drying, which can be accelerated through the use of a drying oven.

### Note!

For gas sterilisation, dry heat, and prior to heating in a microwave oven, all closures and stoppers must be removed as well.

### Heating plastics in microwave ovens

Many plastics are suitable for use in microwave ovens. More accurate information can be obtained from the Table "Physical Properties of Plastics" on page 146. In this connection, it is important to be mindful of the chemical and temperature stability of the various plastics, and to ascertain whether the particular article and its contents are compatible with the given temperature. When aggressive acids, alkalis, or solvents are to be heated, the use of fluoroplastics is recommended. It is very important to provide for adequate ventilation (e.g., fume hoods).

Prior to the use of plastic labware in a microwave oven, the closures and stoppers must be removed from the apparatus.



# Technical information

## Sterilisation\* of plastics

Plastics	Autoclave 121 °C, t <sub>e</sub> 20 min according to DIN	Heated air 160 °C (dry)	Gas (Ethylene oxide)	Chemical (Formalin, ethanol)	β-/γ-radiation 25 kGy
PFA	yes	yes	yes	yes	no
PTFE	yes	yes	yes	yes	no
FEP	yes	yes	yes	yes	no
ETFE	yes	no	yes	yes	no
PMP	yes	no	yes	yes	yes
PP	yes	no	yes	yes	yes (limited)
PE-HD	no	no	yes	yes	yes
PE-LD	no	no	yes	yes	yes
PC	yes <sup>1)</sup>	no	yes	yes	yes
POM	yes <sup>1)</sup>	no	yes	yes	yes (limited)
PA	no	no	yes	yes	yes
SAN	no	no	yes	yes	no
PMMA	no	no	no	yes	yes
PS	no	no	no	yes	yes
PVC	no	no	yes	yes	no
MF	no	no	yes	no	no
NR	no	no	yes	yes	no
SI	yes	-	yes	yes	no
EPDM	yes	-	yes	yes	-
FKM	yes	-	yes	yes	-

\* Before sterilisation, labware must be carefully cleaned and rinsed with distilled water. Always remove covers from containers!

<sup>1)</sup> Frequent autoclaving may reduce mechanical stability!

## Suitability of plastics for foodstuffs



The marked products comply with the lawful regulations of the German Consumer Goods Ordinance and/or Directives (EC) No. 1935/2004, (EC) No. 975/2009 and (EU) No. 10/2011 as amended.

In the testing for compliance with the threshold values for the global migration (or respectively, the specific migration threshold values), no determinations exceeded the allowed values. In addition, sensory testing found no olfactory and flavour-related impairments. The testing was implemented according to the 82/711/EEC and 85/572/EEC Guidelines by an independent, accredited institute.

All source materials used in the manufacturing of the products are listed in the German Consumer Goods Ordinance as at 20.12.2006, or respectively, Directive (EU) 10/2011, in accordance with the present attestation. Therefore, they represent permissible source materials in accordance with food law and may be used in the production of food commodities in accordance with the specified restrictions concerning migration threshold values and permissible residual content in the end product.

Marked PP products are suitable for contact with all foodstuff categories providing that a contact period of 24 hours and a contact temperature of 40 °C are not exceeded. Marked SAN products are suitable for contact with all aqueous, alcoholic and fatty foods, providing that a contact period of 24 hours and a contact temperature of 40 °C are not exceeded.

## Disposal and Recycling of Plastics

If the disposal of a piece of plastic labware is unavoidable, regional laws and regulations must be observed. Recycling centres can be found in many cities, which are designed for the disposal of recyclable materials. To simplify the task of sorting in these recycling centres, the majority of labware from VITLAB can be easily identified and presorted by using the engraved or imprinted recycling code. Prior to disposal, plastic labware must be cleaned, and sterilised if necessary, according to the currently valid regulations.

To simplify the separation of plastics for recycling, so that these can later be reused as raw material for manufacture, plastic identification labels (number 01-07) have been introduced. This identification scheme was published in 1988 under the title "SPI resin identification coding system" by the Society of the Plastics Industry (SPI). For coding, the commonly used shorthand for plastics according to the DIN 7728 is also used.



SPI number 07 stands for "other". This is used to indicate other plastics such as PMP, PFA, PTFE etc. VITLAB doesn't use the "0"; rather, it identifies the specific raw material with the abbreviation according to DIN 7728 to simplify identification of the plastic for the end user.

## CE mark / CE-IVD Guidelines

---

### **IVD Guidelines of the EU**

On 7 December, 1998, the EU "Guidelines for In Vitro Diagnostic Devices" (IVD Guidelines) were published in the Official Journal of the European Communities, and thus came into force. The Guidelines were transposed into German National Law on 1 January, 2002, as a corresponding modification of the German Medical Devices Act (MPG). Consequently, in vitro diagnostic devices are considered medical devices.

### **Definition: Medical devices\***

Medical devices are all instruments, apparatus, devices, materials, or other objects including software that are intended by the manufacturer for use in humans:

- for the purpose of detection, prevention, monitoring, treatment, alleviation or compensation of diseases, injuries or disabilities;
- for the purpose of investigation, replacement or modification of the anatomy or of a physiological process;
- for the purpose of control of conception. Pharmacologically or immunologically active agents are excluded, as these are regulated by the German Pharmaceuticals Law.

### **Definition: In vitro Diagnostic Devices (IVD)\***

"In vitro diagnostic devices" are medical devices that are used for in vitro investigations of samples derived from the human body, including donated blood and tissue. Included are reagents, calibration substances or devices, control substances or devices, equipment, instruments, apparatus, systems, or also sample containers, if they are specifically intended by the manufacturer for use in medical tests. "In vitro diagnostic devices" serve mainly to provide information on:

- physiological or pathological conditions;
- congenital anomalies;
- monitoring of therapeutic measures.

### **CE Mark**

With the CE mark on a product, the manufacturer affirms that the product complies with the requirements for products of that type established by the EU Guidelines and, as necessary, has undergone the required testing. The manufacturer applies this mark to the product and additionally produces a Conformity Declaration that certifies the conformity of the product with the cited guidelines and standards.

The medical products supplied by VITLAB are all included in the class of in vitro diagnostic (IVD) devices.

This includes, for example:

- VITLAB® micropipettes
- Pipette tips
- Urine bottles
- Microtubes

\* See the definitions according to MPG § 3 (Definition of Terms)

## Accuracy

### What do “tolerance, accuracy, coefficient of variation, and precision” mean in volumetric measurements?


#### Graphic illustration of precision and accuracy

The dart board simulates the volume range around the centred nominal value, the white dots simulate the different measured values of a specified volume.

**Good accuracy:** All hits are near the centre, i.e., the nominal value.

**Good precision:** All hits are close together.


**Result:** The manufacturing process is well controlled by an accompanying quality assurance program. Minimal systematic deviations and a narrow variance in products. The permissible limits are not exceeded. There are no rejects.



**Good accuracy:** On average, the hits are evenly distributed around the centre.

**Poor precision:** No substantial errors, but hits widely scattered.


**Result:** All deviations are “equally probable”. Instruments exceeding the permissible tolerance should be rejected.



**Poor accuracy:** Although all hits are close together, the centre (nominal value) is still missed.

**Good precision:** All hits are close together.


**Result:** Improperly controlled production, with systematic deviation. Instruments exceeding the permissible tolerance should be rejected.



**Poor accuracy:** The hits are far removed from the centre.

**Poor precision:** The hits are widely scattered.

**Result:** These volumetric instruments are of inferior quality.



#### Calculation formulae

The accuracy of glass volumetric instruments is commonly defined by “Tolerance Limits”, whereas for liquid handling instruments the statistical terms “Accuracy [%]” and “Coefficient of Variation [%]” have been established.

#### Tolerance

The term “tolerance” (tol.) in the corresponding standards defines the maximum permissible deviation from the nominal value.

$$\text{Tol.} \geq |V_{\text{meas.}} - V_{\text{nom.}}|$$

#### Accuracy

Accuracy (A) indicates the closeness of measured mean volume to the nominal value, i.e., systematic measurement deviation. Accuracy is defined as the difference between the measured mean volume ( $\bar{V}$ ) and the nominal value ( $V_{\text{nom.}}$ ), related to the nominal value in percent.

$$A[\%] = \frac{\bar{V} - V_{\text{nom.}}}{V_{\text{nom.}}} \cdot 100$$

#### Coefficient of Variation

The coefficient of variation (CV) indicates the closeness of values from repeated measurements, i.e., random measurement deviation. The coefficient of variation is defined as standard deviation in percent, related to the mean volume.

$$CV[\%] = \frac{s \cdot 100}{\bar{V}}$$

#### Partial volumes

(analogous to  $CV_{\text{part.}} \%$ )

Generally, A and CV are based on

the nominal volume ( $V_{\text{nom.}}$ ). These data in percent must be converted to partial volumes ( $V_{\text{part.}}$ ). By contrast, there is no conversion for partial volumes if A and CV are stated in volume units (e.g. ml).

$$A_{\text{part.}}[\%] = \frac{V_{\text{nom.}}}{V_{\text{part.}}} \cdot A_{\text{nom.}}\%$$

#### Tolerance from A and CV

To a good approximation, the tolerance, e.g. for the nominal volume ( $V_{\text{nom.}}$ ), can be calculated from the accuracy and coefficient of variation.

$$\text{Tol.} \geq \frac{|A\%| + 2CV\%}{100\%} \cdot V_{\text{nom.}}$$

#### Precision

If the variance in the individual measurement results about the mean volume  $\bar{V}$  is given in units of volume, this relates to precision.

# Cat. No. Index

33331	24	60703	78	66695	81	73598	85	80348	96
33332	24	60795	78	66795	81	73698	85	80375	113
33333	24	60803	78	66895	81	73898	85	80408	109
36491	115	60895	78	66995	81	75991	89	80409	109
39194	60	60903	78	67095	81	76299	123	80410	109
39294	60	60995	78	67104	40	77094	87	80411	109
39394	60	61003	78	67195	40	78294	88	80412	109
39494	60	61095	78	67204	40	78394	88	80413	109
39594	60	61103	78	67295	40	78593	120	80418	120
39694	60	61195	78	67304	40	78794	118	80419	120
39794	60	61203	78	67395	40	79194	52	80434	119
39894	60	61295	78	67404	40	79790	121	80435	119
39994	60	61403	78	67495	40	79890	121	80436	119
40093	61	61495	78	67504	40	79990	121	80437	86
40193	61	61503	78	67595	40	80130	98	80438	86
40293	61	61595	78	67604	40	80131	98	80439	86
40393	61	61603	78	67695	40	80134	98	80440	86
40493	61	61695	78	67704	40	80139	33	80441	86
40593	61	61703	78	67795	40	80140	33	80442	86
40693	61	61795	78	67895	62	80162	86	80443	86
40793	61	61803	78	67995	62	80164	86	80445	86
40894	63	61895	78	68099	62	80165	86	80452	80
41094	63	64091	46	68199	62	80213	123	80454	80
41194	63	64191	46	68299	62	80215	53	80455	80
41294	63	64291	46	68399	62	80217	53	80456	80
41394	63	64391	46	68594	95	80218	53	80459	119
41494	63	64491	46	68894	95	80219	53	80460	119
41594	63	64591	46	69194	95	80221	53	80461	119
41694	63	64604	43	69294	95	80222	53	80462	119
41794	64	64614	43	69394	80	80223	53	80463	119
41894	64	64704	43	69493	80	80229	93	80464	119
41994	64	64714	43	70494	64	80230	92	80465	119
42294	64	64804	43	70594	64	80231	93	80466	119
42393	64	64814	43	70694	64	80252	52	80467	119
42594	116	64891	45	70794	63	80271	90	80468	119
42694	116	64904	43	70894	63	80276	100	80510	118
42794	116	64914	43	70994	63	80277	100	80511	118
42894	116	64991	45	71094	63	80278	100	80512	118
42994	116	65004	43	71194	63	80280	116	80513	118
43094	116	65014	43	71598	121	80281	116	80514	118
43194	116	65091	45	71698	121	80282	116	80515	118
43610	115	65104	43	71798	121	80283	116	80520	119
44091	58	65114	43	71898	121	80284	116	80521	119
44191	58	65191	45	71998	121	80285	116	80525	119
44291	58	65204	43	72098	121	80286	116	80526	119
44391	58	65214	43	72198	121	80288	116	80535	119
44491	58	65291	45	72298	121	80340	96	80536	119
53510	75	65304	43	72398	121	80342	96	80537	119
53610	75	65414	43	72498	121	80343	96	80550	92
60503	78	65965	93	72898	85	80345	96	80551	93
60603	78	65975	93	72998	85	80346	96	80553	93
60695	78	65980	93	73498	85	80347	96	80554	92

80555	93	83312	107	95089	107	104197	97	110304	77
80556	93	83313	107	95093	70	104199	51	110305	76
80557	93	83314	107	95094	106	104297	97	110394	103
80560	97	83315	107	95187	73	104397	97	110404	77
80562	97	83316	107	95188	71	104497	97	110405	76
80593	62	83317	107	95189	107	104597	97	110494	103
80594	62	83330	103	95193	70	104997	97	110594	103
80595	62	90694	112	95194	106	105097	97	110604	77
80596	62	90794	112	95286	75	105197	97	110605	76
80602	115	90894	112	96093	59	105297	97	110704	77
80603	115	90994	112	96293	59	105597	97	110804	77
80604	115	91094	112	96393	59	105599	32	110904	77
80730	95	91194	112	96593	59	105697	97	110905	76
80731	95	91294	112	96694	59	105699	32	111004	77
80732	95	91394	112	96794	59	105799	33	111005	76
80733	95	91494	112	97791	58	105899	33	111194	103
80734	95	91789	109	97891	58	106399	32	112197	77
80735	95	91989	19, 109	99099	100	106499	32	112297	77
80736	95	92089	19, 109	99199	100	106599	32	112397	77
80737	95	92189	19, 109	99299	100	106699	32	112497	77
80828	62	92194	112	100389	110	106799	32	112597	77
80877	118	92489	19, 109	100394	111	106899	32	112697	77
80878	118	92689	109	100489	110	107097	38	112797	77
80879	118	92789	109	100494	111	107197	38	112897	77
80910	94	92889	109	100589	110	107297	38	113197	80
80911	94	93389	107	100594	111	107397	38	113297	80
80952	122	93489	107	100689	110	107497	38	113397	80
80953	122	93788	71	100694	111	107597	38	113497	80
80954	122	93789	107	100789	110	107797	90	122097	84
80970	88	93793	70	100889	110	107897	90	122197	84
80996	52	93794	106	100989	110	107997	90	122297	84
81056	89	93988	71	101589	110	108092	105	122597	106
81213	123	93989	107	101594	111	108192	105	122697	106
81219	53	93993	70	101689	110	108292	105	122797	106
81640	113	93994	106	101694	111	108297	104	122897	106
81642	113	94188	71	101789	110	108392	105	130294	95
81644	113	94189	107	101794	111	108397	104	130297	94
81646	113	94193	70	101889	110	108492	105	130394	95
81660	113	94194	106	101894	111	108497	104	130397	94
81662	113	94587	73	101989	110	108792	70	130494	95
81664	113	94588	71	102089	110	108892	70	130497	94
81666	113	94589	107	102189	110	108992	70	130594	95
83300	72	94687	73	102397	105	109297	104	130597	94
83301	72	94688	71	102597	105	109397	104	131097	120
83302	72	94689	107	102697	105	109497	104	132193	73
83303	72	94987	73	102897	105	109597	104	132293	73
83304	72	94988	71	103297	89	109697	104	132393	73
83306	73	94989	107	103397	89	109797	104	132493	73
83307	73	94993	70	103797	96	110194	103	132593	73
83308	73	94994	106	103897	96	110204	77	132603	71
83310	107	95087	73	104097	97	110205	76	132605	71
83311	107	95088	71	104099	51	110294	103	132606	71

# Cat. No. Index

132608	71	149794	27	300597	82	318597	84	481944	57
132693	73	149893	74	300897	82	319099	25	481945	57
132703	71	149993	74	301097	82	324594	51	482941	57
132705	71	149994	27	301197	82	324694	51	482942	57
132706	71	150094	27	301597	82	324794	51	482943	57
132708	71	150194	28	301697	82	325095	86	482944	57
132793	73	150294	28	301797	82	325195	86	482945	57
132803	71	150394	28	301897	82	325295	86	483941	57
132805	71	151594	114	301997	82	325395	86	484941	57
132806	71	155094	114	302097	82	325495	86	605081	79
132808	71	155400	27	302197	82	326094	92	606081	79
133181	69	155494	27	302297	82	326194	92	606941	79
133281	69	155594	114	302397	82	326294	92	607081	79
133381	69	155600	27	302497	82	326496	92	607941	79
134293	72	155694	27	302597	82	326596	92	608081	79
134393	72	155800	27	303097	82	326696	92	608941	79
134493	72	155894	27	303197	82	395940	60	609081	79
134593	72	155900	28	303297	82	395950	60	609941	79
135181	69	155994	28	307697	83	396940	60	610081	79
135281	69	156094	114	307797	83	396943	60	610941	79
135381	69	159497	91	307897	83	396944	60	611081	79
136693	100	159597	91	307997	83	396946	60	611941	79
138093	108	159665	87	308097	83	396950	60	612081	79
138193	108	159670	87	308197	83	396952	60	612941	79
138293	108	159697	91	308297	83	396955	60	614081	79
138393	108	160110	48	308397	83	396956	60	614941	79
138493	108	160119	48	308497	83	397940	60	615081	79
138593	108	160210	48	308597	83	397950	60	615941	79
138693	108	160219	48	308897	83	406944	61	616081	79
138793	108	160510	48	308997	83	406950	61	616941	79
138893	108	160519	48	309097	83	407944	61	617081	79
139393	108	161010	48	309297	83	407950	61	617941	79
139493	108	161019	48	309397	83	440081	56	618081	79
139593	108	162510	48	310197	84	440941	56	618941	79
139693	108	163094	47	310297	84	441081	56	640941	45
139793	108	163194	47	310397	84	441941	56	641941	45
139893	108	163294	47	310497	84	442081	56	642941	45
145094	99	163394	47	311097	82	442941	56	643941	45
145194	99	163594	47	311197	82	443081	56	644941	45
146294	28	164094	47	311297	82	443941	56	645941	45
146494	28	164194	47	311397	82	444081	56	646081	44
148893	74	164294	47	311497	82	444941	56	646941	44
148894	27	164394	47	311597	82	445081	56	647081	44
148993	74	164494	47	311697	82	445941	56	647941	44
148994	27	164594	47	311797	82	446081	56	648081	44
149093	74	165094	116	316097	83	446941	56	648941	44
149094	27	165194	116	316197	83	447081	56	649081	44
149193	74	165294	116	316297	83	447941	56	649941	44
149194	28	165394	116	316397	83	480941	57	650081	44
149293	74	165494	116	316497	83	481941	57	650941	44
149393	74	165594	116	318293	85	481942	57	651081	44
149693	74	300497	82	318393	85	481943	57	651941	44



652081	44	833089	69	1352939	68	1625506	12	1671682	17
652941	44	833095	69	1352949	68	1625507	12	1671683	17
653081	44	833096	69	1352959	68	1625508	12	1672000	25
653941	44	833098	69	1352969	68	1627515	14	1672002	25
666941	81	833099	69	1352979	68	1627525	14	1672010	25
667941	81	952861	75	1353819	68	1627535	14	1672012	25
668941	81	978081	58	1353839	68	1627545	14	1672015	25
669941	81	978941	58	1353849	68	1630500	50	1672016	25
670040	39	1017940	111	1353859	68	1631500	49	1678132	16
670941	81	1018940	111	1353869	68	1641000	22	1678134	16
670950	39	1037979	96	1431829	67	1641002	22	1678136	16
671040	39	1038971	96	1432829	67	1641004	22	1678210	17
671891	42	1327111	71	1432989	67	1641006	22	1678212	17
671895	41	1328111	71	1433829	67	1641008	22	1678214	17
671941	42	1331819	67	1433959	67	1641010	22	1678216	17
671950	39	1331839	67	1451829	68	1641012	22	1678218	17
672040	39	1331849	67	1452829	68	1670050	25	1678220	17
672891	42	1331859	67	1452989	68	1670066	16, 31	3125970	84
672895	41	1331869	67	1453829	68	1670067	16, 31	3126970	84
672941	42	1332819	67	1453959	68	1670068	16, 31	3190940	98
672950	39	1332839	67	1608000	23	1670072	16	3190941	99
673040	39	1332849	67	1608002	23	1670080	16, 31	3190943	98
673891	42	1332859	67	1608004	23	1670085	31	3190948	98
673895	41	1332869	67	1608006	23	1670095	31	3191940	98
673941	42	1332879	67	1608008	23	1670100	16, 31	3191943	98
673950	39	1332889	67	1610501	18	1670105	16	3191948	98
674040	39	1332899	67	1610502	18	1670110	16, 31	3192940	98
674891	42	1332909	67	1610503	18	1670115	16, 31	3192943	98
674895	41	1332939	67	1610504	18	1670120	16, 31	3192948	98
674941	42	1332949	67	1610506	18	1670125	16, 31	3193940	98
674950	39	1332959	67	1611503	18	1670145	19	3193943	98
675040	39	1332969	67	1611506	18	1670150	16	3193948	98
675891	42	1332979	67	1611508	18	1670155	16, 31	3194940	98
675895	41	1333819	67	1612000	23	1670165	16	3194943	98
675941	42	1333839	67	1612002	23	1670170	16	3194948	98
675950	39	1333849	67	1612004	23	1670175	16	3195940	98
676040	39	1333859	67	1612006	23	1670180	16, 31	3195943	98
676891	42	1333869	67	1612008	23	1670647	50	3195948	98
676895	41	1351819	68	1620506	30	1670648	50	3197940	99
676941	42	1351839	68	1620507	30	1670650	50	3197943	99
676950	39	1351849	68	1621503	13	1670660	50	3197948	99
677891	42	1351859	68	1621504	13	1670702	17	3198940	99
677895	41	1351869	68	1621505	13	1671085	31	3198943	99
677941	42	1352819	68	1621506	13	1671090	15	3198948	99
760941	46	1352839	68	1621507	13	1671095	31	3961111	60
833019	69	1352849	68	1621508	13	1671116	15	4811111	57
833029	69	1352859	68	1622502	13	1671500	15, 31	4821111	57
833039	69	1352869	68	1622504	13	1671505	19		
833049	69	1352879	68	1622505	13	1671506	19		
833085	69	1352889	68	1625503	12	1671510	15, 31		
833086	69	1352899	68	1625504	12	1671515	15		
833088	69	1352909	68	1625505	12	1671520	15		

# Alpha - Index

2-way connector, PE-HD ..... 119

## A

Accessories for VITLAB pipeo® & maneus® ..... 50  
Accessories for VITLAB® microlitre pipettes ..... 25  
Adapter for VITLAB® continuous E/RS ..... 31  
Adapter for VITLAB® dispensers ..... 16  
Adapter for VITLAB® piccolo ..... 19  
Analytical funnels, PP ..... 86  
Autosampler-vials, PFA ..... 97

## B

Beakers ..... 56 - 58, 76 - 80  
Bottle-top burette VITLAB® continuous ..... 30  
Bottle-top dispenser VITLAB® genius<sup>2</sup> ..... 12  
Bottle-top dispenser VITLAB® piccolo ..... 18  
Bottle-top dispenser VITLAB® simplex<sup>2</sup> / simplex<sup>2</sup><sub>fix</sub> ..... 13  
Bottle-top dispenser VITLAB® TA<sup>2</sup> ..... 14  
Bottles ..... 66 - 73, 104 - 113  
Bottles for VITLAB® continuous E/RS ..... 31  
Bottles for VITLAB® piccolo, PE-HD ..... 19  
Bottles, brown glass, for VITLAB® genius<sup>2</sup> / simplex<sup>2</sup> ..... 15  
Bowl, PP, with lid ..... 115  
Bowls, PP ..... 116  
Brown glass bottles for VITLAB® genius<sup>2</sup> / simplex<sup>2</sup> ..... 15  
Büchner funnels, PP ..... 86  
Bucket with spout, PP ..... 59  
Buckets, PE-HD ..... 59  
Bulb pipettes, PP, Class B ..... 47  
Burette clamps, PP ..... 33  
Burette stopcocks, PMP/PTFE ..... 33  
Burette VITLAB® continuous ..... 30  
Burettes, borosilicate glass 3.3 ..... 32  
Burettes, VITLAB® Dr. Schilling ..... 32

## C

Cans ..... 94 - 97  
Caps with dropper inserts, PE-HD ..... 73  
Catchment trays, PP ..... 116  
Chemical waste disposal system, PE/PP ..... 114  
Collectors, PP or SAN ..... 58  
Coloured wash-bottles, PE-LD/PP ..... 71  
Connectors ..... 118, 119  
Connectors, straight, PP ..... 118  
Connectors, T-shape, PP ..... 119  
Connectors, universal PP ..... 118  
Connectors, Y-shape, PP ..... 119  
Container, PP ..... 114  
Coplín staining chamber, PP ..... 100

## D

Desiccator plates, PP and porcelain ..... 93  
Desiccators with stopcock, PC ..... 92  
Desiccators with stopcock, PP/PC ..... 92  
Desiccators, PP/PC ..... 92  
Discharge tubes, flexible for VITLAB® dispensers ..... 16  
Dishes ..... 80, 116, 122  
Dishes, PVC ..... 116  
Dispenser VITLAB® genius<sup>2</sup> ..... 12  
Dispenser VITLAB® piccolo ..... 18  
Dispenser VITLAB® simplex<sup>2</sup> / simplex<sup>2</sup><sub>fix</sub> ..... 13  
Dispenser VITLAB® TA<sup>2</sup> ..... 14  
Dispensing cartridge for VITLAB® TA<sup>2</sup> ..... 17  
Disposable pipettes, PS ..... 48  
Double spatula ..... 62  
Drawer organisers, PVC ..... 122  
Dropping bottles, PE-LD ..... 73  
Dropping bottles, PE-LD/PE-HD ..... 73  
Dropping pipettes ..... 74

Drying racks ..... 123  
Drying tube for VITLAB® continuous E/RS ..... 31  
Drying tube for VITLAB® dispensers ..... 15

## E

Erlenmeyer flasks ..... 81  
Evaporating dishes, PFA ..... 89

## F

Filling tubes for VITLAB® dispensers ..... 17  
Filtering rack ..... 88  
Flexible discharge tubes for VITLAB® dispensers ..... 16  
Forceps ..... 62  
Funnels ..... 63, 64, 86  
Funnels, PP ..... 63

## G

Gas wash bottles, PFA ..... 91  
Graduated beakers, coloured, PP ..... 57  
Graduated beakers, PP ..... 56, 57  
Graduated beakers, SAN ..... 58  
Graduated beakers, stackable, PP ..... 57  
Graduated cylinders, PMP, Class A, tall shape ..... 43  
Graduated cylinders, PP, Class B, short shape ..... 45  
Graduated cylinders, PP, Class B, tall shape ..... 44  
Graduated cylinders, SAN, Class B, short shape ..... 46  
Graduated cylinders, SAN, Class B, tall shape ..... 45  
Graduated pipettes ..... 47, 48  
Graduated pipettes, PP, Class B ..... 47  
Griffin beakers, ETFE ..... 77  
Griffin beakers, PFA ..... 76  
Griffin beakers, PMP ..... 78  
Griffin beakers, PP ..... 79  
Griffin beakers, PTFE ..... 77

## H

Hydrometer cylinder, PP ..... 46

## I

Imhoff cone, SAN ..... 89

## L

Lab bottles VITgrip™, PP, GL 45 ..... 102, 103  
Laboratory trays, PP ..... 116  
Large funnels, PE-HD ..... 64  
Large funnels, PP ..... 64  
Lids for trays, PS ..... 121

## M

Magnetic stir bar, triangular, PTFE ..... 84  
Magnetic stir bars ..... 82 - 84  
Magnetic stirring bar retrievers, flexible, PTFE ..... 84  
Magnetic stirring bar retrievers, PE ..... 85  
Magnetic stirring bar retrievers, PTFE ..... 84  
Magnetic stirring bars, barbell, PTFE ..... 84  
Magnetic stirring bars, cross shape, PTFE ..... 83  
Magnetic stirring bars, octagonal, PTFE ..... 83  
Magnetic stirring bars, oval, PTFE ..... 82  
Magnetic stirring bars, polygonal, PTFE ..... 82  
maneus® ..... 50  
Measuring cup, PP ..... 80  
Measuring scoops, coloured, PP ..... 60  
Measuring scoops, PP ..... 60  
Microlitre pipettes ..... 22, 23  
Microtube stands ..... 99  
Microtubes, PP ..... 99  
Mortars, MF ..... 85  
Multi-channel pipettes ..... 23  
Multi-purpose container, SAN ..... 115

**N**

Narrow-mouth bottles	104 - 109
Narrow-mouth bottles, PE-HD	109
Narrow-mouth bottles, PE-LD	107, 108
Narrow-mouth bottles, PFA	104
Narrow-mouth bottles, PP	106
Non-return valves	120

**O**

O-rings for desiccators	93
-------------------------	----

**P**

Pasteur pipettes	74
Pestles, MF	85
PFA-economy narrow-mouth bottles	105
PFA-economy wash bottles	70
pipeo®	49
Pipette baskets	53
Pipette fillers	51
Pipette jars	53
Pipette stands	52
Pipette tips, PP	26 - 28
Pipette trays	52
Pipette washer	53
Pipettes	47, 48, 74
Pipettes, Piston-operated pipettes	22, 23
Piston-operated pipettes	22, 23
Plastic stand for VITLAB® dispensers	15
Powder funnels, PP	63
PTFE-tape	120

**R**

Reagent bottles, opaque, PP, wide mouth	111
Reagent bottles, PP	110, 111
Reagent reservoir	25
Reagent tube racks	97, 98
Round-bottom flask stand	90
Round-bottom flasks, PFA	90

**S**

Safety wash bottles, VITsafe™	66 - 72
Sample containers	94 - 97
Sample containers, PE-HD	94
Sample containers, PE-LD	95
Sample containers, PFA	94
Sample containers, PP	95
Sample tubes, PFA	96
Sample vials, PFA	97
Scoops	60, 61
Scoops, PE-HD	61
Screw caps, PFA	105
Screw caps, PP	107
Sealing ring for the valve block for VITLAB® dispensers	17
Sealing tape, PTFE	120
Sedimentation cone, SAN	89
Sedimentation rack	89
Slide storage boxes, PS	100
Spatula	62
Spatula spoon	62
Spray bottles	75
Spray bottles, PP	75
Staining chamber for slides, POM	100
Staining jar for slides, POM	100
Staining rack for slides, POM	100
Standard joint funnels, PP	64
Standard joint stoppers, PP	112
Starter-Sets VITLAB® micropipette	24

Stir bars, magnetic	82 - 84
Stirring rod, PP	62
Stopper, PP, Standard joint	112
Storage bottles, PE-HD, with tap	113
Storage bottles, PE-HD, without tap	113
Support for separatory funnels	88

**T**

Tap for storage bottles, PP	113
Telescopic filling tube for VITLAB® continuous E/RS	31
Telescopic filling tubes for VITLAB® dispensers	17
Test tube racks, coloured, PP	98
Threaded bottles for VITLAB® continuous E/RS	31
Tip-Box	26
Transport container, PE-HD	115
Trays, MF	121
Tubing connectors	118, 119

**U**

Urbanti funnels, PMP	86
----------------------	----

**V**

Valve for desiccators	93
VENT-CAP wash bottle caps	69
Ventilation plug for micro filter for VITLAB® genius <sup>2</sup> / simplex <sup>2</sup>	17
VITgrip™ lab bottles, PP, GL 45	102, 103
VITLAB maneus®	50
VITLAB maneus® pipette helper	50
VITLAB pipeo®	49
VITLAB pipeo® pipette helper	49
VITLAB® continuous E/RS	30
VITLAB® Dr. Schilling burettes	32
VITLAB® genius <sup>2</sup>	12
VITLAB® micropipette -8/-12	23
VITLAB® micropipette Starter-Sets	24
VITLAB® micropipettes	22
VITLAB® opaque volumetric flasks, PMP, Class A	39
VITLAB® piccolo	18
VITLAB® simplex <sup>2</sup> / simplex <sup>2</sup> <sub>fix</sub>	13
VITLAB® TA <sup>2</sup>	14
VITsafe™ safety wash bottles, narrow-mouth	67
VITsafe™ safety wash bottles, wide-mouth	68
Volumetric flasks, PFA, Class A	38
Volumetric flasks, PMP, Class A	40
Volumetric flasks, PMP, Class B	40, 41
Volumetric flasks, PP, Class B	42

**W**

Wash bottle caps, PP	72
Wash bottle caps, VENT-CAP	69
Wash bottles with imprint, PE-LD/PP	69
Wash-bottles	66 - 72
Wash-bottles, PE-LD	72
Wash-bottles, PE-LD/PP	71
Wash-bottles, PP	70
Wash-bottles, VITsafe™	66 - 72
Watch glasses, PP	80
Watch glasses, PTFE	80
Water-jet pump, PP	87
Weighing jars, PP	96
Wide-mouth bottles	104, 106 - 109
Wide-mouth bottles, PE-HD	109
Wide-mouth bottles, PE-LD	107 - 109
Wide-mouth bottles, PE-LD, with eye closure	109
Wide-mouth bottles, PFA	104
Wide-mouth bottles, PP	106
Wide-mouth bottles, PTFE	106

# General Terms and Conditions of VITLAB GmbH

## 1. General

- 1.1 These General Terms and Conditions (GT&C) are intended for use in commercial transactions between businesses.
- 1.2 These GT&C shall apply for all, including future, contracts with the customer. Other terms and conditions shall not become part of the contract, even if VITLAB does not expressly object to them. Amendments to and changes of the contract must be in written form. The waiver of the requirement for written form shall only be possible in writing. This shall not apply to individual contractual agreements. The language of the contract shall be German and/or English. In the event of a discrepancy between the German language version of these GT&C and a version in any language, the German language version shall prevail.
- 1.3 VITLAB offers are subject to change and non-binding. VITLAB reserves the right to make technical improvements to VITLAB products.
- 1.4 VITLAB may electronically store and process data necessary for the purpose of processing the contract.
- 1.5 A set-off by the customer shall not be permitted unless the counterclaims are undisputed or legally established, or pecuniary counterclaims arising from the right to refuse payment pursuant to Section 320 Bürgerliches Gesetzbuch (BGB) (German Civil Code).
- 1.6 Orders with a goods value of below € 250 shall be subject to a minimum order surcharge of € 50. Delivery shall be undertaken generally in packaging units (PU) according to the currently valid price list. For deliveries within five (5) working days or for order values up to € 500, VITLAB reserves the right to waive an order confirmation.
- 1.7 For commercial transactions with customers having no general place of jurisdiction in Germany and between businesses, public law persons or special funds under public law the place of jurisdiction shall be the court responsible in Aschaffenburg, Germany. VITLAB shall also be entitled to appeal to the court responsible for the head office of the customer. VITLAB shall, furthermore, as plaintiff have the right to invoke the Arbitration Court at the Chamber of Commerce and Industry in Frankfurt am Main, Germany. The Arbitration Court shall, in this case, make the final judgment in accordance with the Rules of Arbitration of the Chamber of Commerce and Industry in Frankfurt am Main without recourse to the ordinary courts of law. The instigation of legal dunning proceedings by VITLAB shall not signify the exertion of its right of choice; it shall be admissible in all cases.
- 1.8 German law shall apply exclusively under the exclusion of the conflict of laws principles of Private International Law and the UN Convention on Contracts for International Sale of Goods (CISG).

## 2. Delivery

- 2.1 The place of performance shall be the factory of VITLAB in Großostheim, Germany. The risk shall transfer to the customer when the goods for delivery are packed and ready for pick-up (EXW (Incoterms® 2010 ex works)). This shall also apply to partial deliveries or where VITLAB has performed additional services, such as shipping; costs for transport, packaging or insurance; exportation and installation. This shall also apply in case of delivery to a consignment warehouse of the customer.
- 2.2 Insofar as VITLAB has agreed to orders on call, the customer must take delivery prior to the agreed date, otherwise within six (6) months.

## 3. Delivery Period, Delay

- 3.1 Delivery times shall be ex works. Delivery periods shall begin on receipt of our order confirmation by the customer; however only after settlement of any technical issues pending from the conclusion of the contract; and after receipt of any documents to be provided to VITLAB by the customer, such as drawings, permits or approvals; and definitely not before receipt of agreed advance payments. The delivery period shall be considered to have been met if readiness for dispatch has been notified before the expiry of this period. Delivery shall be subject to VITLAB receiving its own supplies punctually and in good order.
- 3.2 Force Majeure and circumstances beyond control of VITLAB, such as strikes, lock-outs, operational disruption, shortages of raw materials and equipment, delayed delivery or non-delivery by VITLAB suppliers, shall extend the delivery periods accordingly and shall release VITLAB from its delivery obligations if they, as a result, render delivery impossible. VITLAB shall also not be liable for the circumstances described above if they arise during an already existing delay. The same shall apply for any additional or amended services requested by the customer.
- 3.3 VITLAB shall be considered to be in default of delivery only if the customer has issued VITLAB with a reminder, has set a reasonable extension period which has elapsed. The customer shall be obliged to immediately inform VITLAB in writing of any likely consequences of delay.
- 3.4 In the case of delay damages, VITLAB's liability for compensation shall be limited to 10% of the value of the delayed delivery/service. The limitation shall not apply in cases of willful intent, gross negligence and/or injury to life, limb or health.

## 4. Prices, Terms of Payment

- 4.1 Prices shall be EXW (Incoterms® 2010 ex works) Großostheim and exclusive of statutory VAT, if applicable. Costs of packaging, transportation, freight and insurance shall be borne by the customer. Prices shall also be exclusive of the cost of returning and recycling/disposing of old equipment.
- 4.2 Invoices shall be payable to VITLAB account in EUROS (€) without deductions and free of charges and expenses. Payment shall be made immediately or by the date stated. The determinant factor shall be the receipt of payment. Cheques and bills of exchange shall only be accepted on account of performance and at the cost of the customer.
- 4.3 In the case of customers, with whom VITLAB is working for the first time or with whom VITLAB does not work regularly, after delay in payment or in the case of reasonable doubt as to the creditworthiness of the customer, VITLAB shall reserve the right to make individual deliveries dependent on a pre-payment or a security deposit to the value of the invoice amount.
- 4.4 Should the period between conclusion of contract and agreed delivery exceed four (4) months, so may VITLAB, at its discretion, demand a reasonable additional charge equivalent to the increase in its costs up until delivery. 4.5 In the case of an agreed return of goods that are free of defects, the customer shall be charged a checking and processing fee of 20 % of the invoice amount (minimum € 50).
- 4.6 Should the customer be in arrears with payment, VITLAB debt claims against him shall be due immediately, and VITLAB shall not be obliged to make any further deliveries based on current delivery contracts.
- 4.7 If payment is delayed, VITLAB shall charge – notwithstanding further damage compensation claims – interest on arrears at the statutory rate.
- 4.8 VITLAB may offset amounts payable to the customer (e.g. from credit notes) against VITLAB claims against the customer.

## 5. Retention of Title, Assignment of Future Claims

- 5.1 The goods delivered shall remain property of VITLAB until the complete and unconditional payment. Should VITLAB still have further claims against the customer arising from the business relationship, VITLAB shall then retain its property rights until payment of such claims has been effected.
- 5.2 The customer may neither use goods subject to retention of title nor combine them with other objects to which a third party may have rights. Should, however, goods subject to retention of title become, through their combination with other objects, part of a new (complete) item, VITLAB shall be a proportional co-owner of this new item directly, even if this latter component is regarded as the main component. VITLAB'S proportion of co-ownership shall be determined by the ratio of the invoice value of the goods to the value of the new item at the time of combination.
- 5.3 The customer may resell goods subject to retention of title in the course of his normal business as long as he has not assigned, pledged or otherwise encumbered his claims from the resale.
- 5.4 The customer shall assign to VITLAB in advance as collateral any claims against his customers from the resale of the goods subject to retention of title (see Clause 5.3) and/or newly formed items (see Clause 5.2) to the value of VITLAB'S invoice for the goods subject to retention of title. As long as the customer is not in default of payment for the goods subject to retention of title, he may collect the assigned claims in the ordinary course of business. He may, however, only use the proportional proceeds for the payment to VITLAB for the goods subject to retention of title.
- 5.5 At the customer's request, VITLAB shall release collateral at its discretion if and to the extent that the nominal value of the collateral exceeds 120% of the nominal value of our outstanding debt claims against the customer.

- 5.6 The customer shall be required to inform VITLAB immediately of any attachments, seizures or any other third-party dispositions relating to the goods that are reserved or co-owned by VITLAB.
- 5.7 In the event of delay in payment, failure to pay bills of exchange or cheques, or failure or recall of a payment made via SEPA Direct Debit Scheme, suspension of payments or insolvency of the customer or of the end buyer, the rights of the customer under Clause 5.3 shall no longer be valid. The customer must then immediately inform the buyer of VITLAB'S extended retention of title; he may use the proportional proceeds relating to the assignment only to pay for the delivered goods. VITLAB shall be entitled to collect the assigned receivables itself.
- 5.8 In the event of customer's culpable breach of contractual obligations, in particular for the cases covered in Clause 5.7, VITLAB shall be entitled to withdraw from the contract and/or, without withdrawing from the contract, demand the return of any goods subject to retention of title still in possession of the customer and to collect the assigned receivables itself. In order to ascertain the rights of VITLAB, VITLAB shall be entitled to have all of customer's documents/books concerning the reserved rights examined by a person who is subject to the professional duty of confidentiality.

## 6. Warranty, Limitation of Liability

- 6.1 VITLAB warrants that its delivered goods (including any agreed installation) are free of defects at time of risk transfer. The required quality, durability and use of VITLAB'S delivered goods are based solely on the agreed written specification, product description and/or operating manuals. Any information beyond this, in particular in preliminary discussions, advertising and/or referencing industrial standards shall only become part of the contract if they are expressly referenced in writing.
- 6.2 Should the customer require the delivered goods for purposes other than those agreed, he must take responsibility himself for examining their special suitability for this – also in terms of product safety – and ensure their compliance with all relevant technical, legal or regulatory provisions before the intended use. VITLAB shall not be liable for any usability that was not expressly confirmed by VITLAB in writing. In the case of material or design requirements of the customer, VITLAB shall accept no liability for the suitability or permissibility of the desired materials or designs. Compliance with safety-related and occupational health regulations depends on the location and operating conditions of which VITLAB has no prior knowledge. Action for ensuring compliance shall therefore be the responsibility of the customer or his buyer.
- 6.3 VITLAB shall not be liable for the consequences of improper handling, use, maintenance and operation of the delivered goods; the consequences of normal wear and tear, in particular of wearing parts, such as pistons, seals, valves; the breakage of glass, plastic or ceramic parts; for the consequences of chemical, electrochemical or electrical influences; or non-observance of the operating instructions.
- 6.4 If a notice of defect is justified, VITLAB shall initially only be required to provide cure. Any such cure shall be, at the discretion of VITLAB, either rectification of the defect or delivery of goods free of defects. Further warranty claims shall only apply in the event of rejection, impossibility or failure of the cure. If cure is possible only at disproportionate expense pursuant to Section 439 Para. 4 BGB (German Civil Code), VITLAB will bear the cost necessary for the cure according to Section 439 Para. 2, 3 BGB (German Civil Code) up to a limit of 150 % of the value of the delivered goods free from defects.
- 6.5 The customer must, immediately upon receipt of the goods, inspect them carefully, also in terms of product safety, and notify obvious defects immediately in writing; any hidden defects must be immediately notified upon discovery. The customer must notify the carrier immediately of any transport damage. Failure to observe the testing and notification obligation shall void any customer claims for defects.
- 6.6 VITLAB'S liability for slight negligence shall be limited to claims for injury to life, limb or health, to claims under the Produkthaftungsgesetz (German Product Liability Act) or to claims of culpable breach of fundamental contractual obligations through which the purpose of the contract is endangered. Otherwise, our liability for slightly negligent breach of fundamental contractual obligations is limited to the typically occurring damages which VITLAB could have foreseen when the contract was concluded.
- 6.7 Should the customer use the delivered goods in conjunction with environmentally harmful, toxic, radioactive or otherwise hazardous materials, he must notify VITLAB about any such materials and decontaminate the delivered goods prior to returning them to VITLAB. If applicable, VITLAB may charge any necessary costs for decontamination/cleaning and disposal to the customer's account.

## 7. Limitation Period

- 7.1 The warranty period shall be one year and starts from the date of delivery of the goods to the customer. This shall also apply for rights of recourse pursuant to Section 445a BGB (German Civil Code). The same shall apply for claims for damages, irrespective of their legal basis. The limitation periods of Section 438 Para. 1 Nos. 1 and 2 and Section 634a Para. 1 No. 2 of the BGB (German Civil Code) shall remain unaffected. The restriction of the limitation period shall not apply to claims based on fraudulent concealment of a defect, for claims under the Produkthaftungsgesetz (German Product Liability Act) or for damages resulting from injury to life, limb or health and other damages based on intent or gross negligence. The limitation period in respect of replaced or repaired goods shall only commence anew if VITLAB admitted the defectiveness of the replaced or repaired goods.

## 8. Software Use

- 8.1 If software is included in the scope of a delivery, the customer shall be granted a non-exclusive right to use the software and its associated documentation. It is provided for use on the designated delivery item. The use of the software on more than one system shall be prohibited.
- 8.2 The customer shall only be entitled to copy, transfer or translate the software or to convert it from object code to source code to the extent permitted by law (Sections 69a et seq. Urheberrechtsgesetz – German Copyright Act). The customer undertakes to refrain from removing manufacturer information, in particular copyright notices, or from changing these without VITLAB'S prior express consent or the prior express consent of the software supplier.
- 8.3 All other rights to the software and the documentation including copies thereof shall remain with VITLAB and/or the software supplier. The issue of sublicenses is not permitted.

## 9. Spare Parts, Maintenance/Repair and Calibration

- 9.1 For spare parts and maintenance, repair and calibration services, the current repair service and spare parts price list shall apply.
- 9.2 Insofar as there is an obligation on the part of VITLAB to maintain/supply spare parts, then this obligation shall be limited to a period of five (5) years from the date of delivery. If spare parts are not manufactured by VITLAB, or are no longer available on the market, for example electronic components, or if the raw material for their production is no longer available, the obligation of VITLAB to deliver spare parts shall lapse.
- 9.3 For calibration and maintenance, expendable items from VITLAB production are normally used.
- 9.4 Maintenance and calibration services can only be provided if the customer has declared the devices sent to be safe to work on from a health hazard perspective.
- 9.5 For repair/service values of up to € 50, VITLAB reserves the right not to provide a separate cost estimate.

## 10. Legal Reservation, Industrial Property Rights, Confidentiality

- 10.1 VITLAB reserves ownership and all industrial property rights and copyrights to all moulds, tools or other devices, samples, pictures, and business and technical documents produced or provided by VITLAB. This also applies where the customer has wholly or in part taken on the costs hereof. The customer may use these only in the manner agreed with VITLAB. Without VITLAB'S written consent, the customer may not himself manufacture contractual objects delivered or have the same manufactured by third parties.
- 10.2 Insofar as VITLAB delivers goods according to the designs or other requirements specified by the customer (models, patterns etc.), the customer shall be liable to VITLAB by default for ensuring that, through the manufacture and delivery of these goods, the industrial property rights or other rights of third parties are not infringed. If the customer is at fault he shall reimburse VITLAB all damage resulting from any such infringement of rights.
- 10.3 Any information acquired from this business relationship and not deemed to be public knowledge must not be disclosed by the customer to third parties.

Status as of: January 2018

**VITLAB GmbH**

Linus-Pauling-Str. 1  
63762 Grossostheim  
Germany  
tel: +49 6026 9 77 99-0  
fax: +49 6026 9 77 99-30  
e-mail: [info@vitlab.com](mailto:info@vitlab.com)  
[www.vitlab.com](http://www.vitlab.com)

**USt.-IdNr. / VAT REG NO**

DE 1116669 59

WEEE-Reg.-Nr. DE 30031601

**Banking details**

Sparkasse Aschaffenburg  
Deutsche Postbank AG  
Commerzbank AG  
Deutsche Bank AG

**IBAN**

DE91 7955 0000 0000 0003 15  
DE71 5001 0060 0040 0016 06  
DE63 7908 0052 0309 9404 00  
DE49 5087 0005 0010 5619 00

**SWIFT-BIC**

BYLA DE M1 ASA  
PBNK DE FF  
DRES DE FF 790  
DEUT DE FF 508